

SKOOT

DN0047 Rev 08.1
Automated Scanner

SAFETY WARNINGS / PRECAUTIONS

KEEP THIS MANUAL – DO NOT LOSE

THIS MANUAL IS PART OF THE **SKOOT** SYSTEM AND MUST BE RETAINED FOR THE LIFE OF THE PRODUCT. PASS ON TO SUBSEQUENT OWNERS.

Ensure any amendments are incorporated with this document.



WARNING! The SKOOT is designed for a specific use. Using the SKOOT outside of its intended use is dangerous. Failure to comply with the warnings, instructions, and specifications in this manual could result in **SEVERE INJURY** or **DEATH**. Read and understand this manual before using.



WARNING! FALLING OBJECT HAZARD. The area below a crawler must be kept clear at all times. A clearly marked **NO ENTRY ZONE** must be cordoned off directly below the area of crawler operation.

(see Preparation for Safe Use on page 35 for additional details)

WARNING! Do **NOT** operate or place crawler on a surface higher than 2 m (6 ft) without a proper tether held taut at all times.

(see Tether Requirements and Attachment on page 36 for additional details)



WARNING! ELECTRICAL CORDS CAN BE HAZARDOUS.

Misuse can result in **FIRE** or **DEATH** by **ELECTRICAL SHOCK**. Inspect thoroughly before each use. Do **NOT** use if damaged. Do **NOT** use when wet. Keep away from water. Do **NOT** drive, drag or place objects over cord.



WARNING! Do **NOT** operate scanner in an explosive environment. Do **NOT** operate scanner in the presence of volatile substances.





WARNING! MAGNETIC MATERIAL. The wheels of the crawler produce an extremely strong magnetic field which may cause failure or permanent damage to items such as watches, memory devices, CRT monitors, medical devices or other electronics.



Tools, magnets and metal objects can cut, pinch or entrap hands and fingers. **HANDLE WITH CARE.**

People with pacemakers or ICD's must stay at least 25 cm (10 in) away.

WARNING! MAGNETIC MATERIAL. The installation/removal mat (see "Installation/Removal Mat" on page 29) contains magnetic material.

People with pacemakers or ICD's must stay at least 10 cm (4 in) away.



WARNING! LASER RADIATION. The battery powered optical guide contains a Class 1M laser. Do not view directly with optical instruments.



WARNING! If this product is to be used with any Child Products listed in (Chapter 2.3), be sure to read and comply with the warnings, instructions, and specifications in the Child Product's User Manual(s).




WARNING! DO NOT DISASSEMBLE. No user-serviceable parts. Disassembling any of the components in this product, beyond the instructions in this user manual, could void the regulatory certifications and/or effect the safety of the product.



CAUTION! DO NOT operate the SKOOT crawler on an inspection surface which is electrically connected to a component that is being welded.



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.





EMERGENCY STOP. This symbol indicates emergency stop button.



The WEEE symbol indicates that the product must not be disposed of as unsorted municipal waste, but should be collected separately.

(see Disposal on page 135 for additional details).

TABLE OF CONTENTS

1	Identification	3
	1.1. Product Brand	3
	1.2. Manufacturer	3
	1.3. Compliance Declarations	3
	1.3.1. ISED Emissions Compliance (Canada).....	3
	1.3.2. FCC Suppliers Declaration of Conformity (United States).....	3
	1.3.3. European Union CE Declarations	4
2	Product Specifications	5
	2.1. Base SKOOT System	5
	2.1.1. Intended Use	5
	2.1.1.1 Operating Limits	6
	2.1.1.2 Operating Environment	7
	2.1.1.3 User	7
	2.1.2. Unintended Use	8
	2.1.3. Dimensions and Weight	8
	2.1.4. Power Requirements	10
	2.1.5. Environmental Sealing	10
	2.1.6. Performance Specifications	10
	2.1.7. Encoder Interface Specifications	11
	2.2. Compatible Components	12
	2.2.1. Low Profile Probe Holder Frame	12
	2.2.1.1 Intended Use	12
	2.2.1.2 Operating Limits	12
	2.2.2. Vertical Probe Holder Frame	12
	2.2.2.1 Intended Use	12
	2.2.2.2 Operating Limits	12
	2.2.3. Pivoting Probe Holder Frame	13
	2.2.3.1 Operating Limits	13
	2.2.4. Frame Bar.....	13
	2.2.4.1 Intended Use	13
	2.2.4.2 Operating Limits	13
	2.2.5. Slip Joint Probe Holder	14
	2.2.6. Vertical Probe Holder	14

2.2.7.	Heavy Duty Vertical Probe Holder.....	14
2.2.8.	Corrosion Thickness Probe Holder	14
2.2.9.	HydroFORM Cart with Wheels	14
2.2.10.	Preamp Bracket.....	15
	2.2.10.1 Intended Use	15
	2.2.10.2 Operating Limits	15
2.2.11.	Battery Powered Optical Guide	15
	2.2.11.1 Intended Use	15
	2.2.11.2 Operating Environment	15
	2.2.11.3 Power Requirements	15
	2.2.11.4 Environmental Sealing	15
2.2.12.	Medium Temperature Add-On Kit	16
	2.2.12.1 Intended Use	16
	2.2.12.2 Operating Limits	16
2.2.13.	Encoder Adapter	16
	2.2.13.1 Intended Use	16
2.3.	Child Products	17
2.3.1.	Motorized Couplant Pump	17
2.3.2.	Motorized Raster Arm	17
2.3.3.	Optical Guide	17

3

Definitions 18

3.1.	Definition of Symbols	18
3.2.	Definitions of Terms	18
3.3.	Safety Symbols	19
3.4.	Safety Signal Words	19

4

System components 20

4.1.	Component Identification	20
	4.1.1. Base System	20
	4.1.2. Compatible Components	21
	4.1.3. Child Products	23
4.2.	Tools.....	24
	4.2.1. Included Tools	24
	4.2.2. Optional tools	24
4.3.	Base System Components	25
	4.3.1. Crawler	25
	4.3.1.1 Emergency Off Button	25
	4.3.2. Power Controller	26
	4.3.2.1 AC/DC Power Supply	27

4.3.3.	Handheld Controller	28
4.3.4.	Auxiliary Cable	29
4.3.5.	Encoder Cable	29
4.3.6.	Installation/Removal Mat	29
4.3.7.	Lifting Sling	30
4.3.8.	Irrigation Kit	30
4.3.9.	Cable Management	30
4.3.10.	Tools	30
4.3.11.	Cases	30
4.4.	Compatible Components	31
4.4.1.	Low Profile Probe Holder Frame	31
4.4.2.	Vertical Probe Holder Frame	31
4.4.3.	Pivoting Probe Holder Frame	31
4.4.4.	Frame Bar	31
4.4.5.	Slip Joint Probe Holder	31
4.4.6.	Vertical Probe Holder	32
4.4.7.	Heavy Duty Vertical Probe Holder	32
4.4.8.	Corrosion Thickness Probe Holder	32
4.4.9.	HydroFORM Cart	32
4.4.10.	Preamp Bracket	32
4.4.11.	Battery Powered Optical Guide	33
4.4.12.	Automated Crawler Medium Temperature Add-On Kit	33
4.4.13.	Encoder Adapter	33
4.5.	Child Products	34
4.5.1.	Motorized Couplant Pump	34
4.5.2.	Motorized Raster Arm	34
4.5.3.	Optical Guide	34

5

Preparation for Use35

5.1.	Preparation for Transportation	35
5.2.	Preparation for Safe Use	35
5.2.1.	No Entry Fall Zone	35
5.2.2.	Tether Requirements and Attachment	36
5.2.3.	Lifting Sling Setup	37
5.3.	Preparation of Inspection Surface	37
5.4.	System Connectivity	38
5.5.	Configurations	40
5.5.1.	Crawler with Multiple Probe Holders	40
5.5.1.1	Vertical Probe Holder Frame	40
5.5.1.2	Low Profile Probe Holder Frame	42
5.5.1.3	Pivoting Probe Holder Frame	44

	5.5.1.4 Pivoting Probe Holder Frame	46
5.6.	Crawler	48
	5.6.1. Swivel Mount	48
	5.6.2. Umbilical	49
	5.6.3. Handle	50
	5.6.4. Emergency Off Button	51
	5.6.5. Cable Retainer	51
	5.6.6. Manipulation Handle	52
5.7.	Backpack	53
	5.7.1. Mounting a Backpack	53
	5.7.2. Using the backpack	54
5.8.	Probe Holders	55
	5.8.1. Heavy Duty Vertical Probe Holder	55
	5.8.1.1 Probe Holder Setup	55
	5.8.1.2 Probe Holder Vertical Adjustment	57
	5.8.1.3 Probe Holder Left/Right Conversion	58
	5.8.1.4 Probe Holder 90° Adjustment	59
	5.8.2. Vertical Probe Holder	60
	5.8.2.1 Probe Holder Setup	60
	5.8.3. Probe Holder Vertical Adjustment	61
	5.8.4. Probe Holder Transverse Adjustment	62
	5.8.5. Probe Holder Longitudinal Adjustment	63
	5.8.6. Probe Holder Left/Right Conversion	64
5.9.	Slip Joint Probe Holder	66
	5.9.1. Probe Holder Setup	66
	5.9.2. Probe Holder Adjustment	68
	5.9.3. Probe Holder Force Adjustment	68
	5.9.4. Slip Joint Probe Holder Left/Right Conversion	70
5.10.	Probe Holder Frames	72
	5.10.1. Low Profile Probe Holder Frame - Flat or Circumferential Only	72
	5.10.2. Vertical Probe Holder Frame - Flat or Circumferential Only	76
	5.10.3. Pivoting Probe Holder Frame	80
	5.10.3.1 Mounting a Pivoting Probe Holder Frame	81
	5.10.4. Pivoting Probe Holder Frame Setup - Longitudinal Scanning	82
	5.10.4.1 Longitudinal Scanning	82
	5.10.4.2 Circumferential Scanning	83
	5.10.4.3 Pivoting Probe Holder Frame - Flange Scanning	84
	5.10.5. Optical Guide Pivot Mount	87
5.11.	Accessories	88
	5.11.1. Battery Powered Optical Guide	88
	5.11.2. Cable Management	89
	5.11.2.1 Mounting the Cable Management	89

5.11.2	Cable Management Setup	89
5.11.2.3	Clamp Setup	90
5.11.3.	Preamp Bracket	91

6	Operation	92
6.1.	System Startup	92
6.2.	Placement of Crawler on Inspection Surface	94
6.2.1.	Scanner Installation/Removal Mat Use.....	95
6.3.	Operation	97
6.3.1.	Handheld Controller Layout	97
6.3.1.1	Touchscreen	97
6.3.1.2	Click Wheel	98
6.3.1.3	Joysticks	98
6.3.2.	Mode Select Screen	98
6.3.3.	Jog Mode	99
6.3.4.	Latched Jog Mode	101
6.3.5.	System Utilities Screen	102
6.3.5.1	User Settings Screen	102
6.3.5.2	Diagnostics Screens	104
6.3.5.2.1	Detected Modules.....	105
6.3.5.2.2	System 1.....	105
6.3.5.2.3	System 2.....	106
6.3.5.2.4	System 3.....	106
6.3.5.2.5	Skoot-L, Raster.....	107
6.3.5.3	Touch Calibration Screen	108
6.3.5.4	Joystick Calibration Screen	109
6.3.5.5	Draw	110
6.3.6.	High Internal Temperature Screen	110

7	Maintenance.....	111
7.1.	Safety Precautions Before Maintenance	111
7.2.	Cleaning	111
7.3.	Maintenance Schedule	112

8	Troubleshooting	113
8.1.	Startup Issues	113
8.1.1.	Joystick Off Center	113
8.1.2.	Checking Network	113
8.2.	Startup Override	114
8.2.1.	Scan Devices	115
8.2.2.	Reset Parameters	116
8.2.3.	System Parameters	116

8.2.4. Device Address.....	116
8.3. Additional Issues	117
8.4. Retrieval of a Stranded Crawler	118

9 Service and Repair	119
9.1. Technical Support	119

10 Spare Parts	120
10.1. SKOOT Crawler	120
10.2. SKOOT Kit Components	121
10.2.1. Encoder Connector Type	122
10.2.2. Power Cord Type	122
10.3. Probe Holder Frame	123
10.4. Low Profile Probe Holder Frame	124
10.5. Pivoting Probe Holder Frame	125
10.6. Slip Joint Probe Holder Parts	126
10.7. Vertical Probe Holder Parts	127
10.8. Heavy Duty Vertical Probe Holder	128
10.9. Corrosion Thickness Probe Holder	129
10.10. Probe Holder Components	130
10.10.1. Arm Style	130
10.10.2. Yoke Style	130
10.10.3. Swing Arm Style	130
10.10.4. Heavy Duty Yoke Style	130
10.10.5. Pivot Button Style	130
10.10.6. Probe Holder Receptacle and Wear Plate	131
10.11. Variable Components	131
10.11.1. Frame Bar	131
10.11.2. Cable Management Sleeving	131
10.12. Accessories.....	132
10.12.1. Automated Crawler Medium Temperature Add-On Kit	132
10.12.2. Preamp Bracket	133
10.12.3. Battery Powered Optical Guide	133
10.13. Cases	134

11 Disposal	135
--------------------------	------------

12 Limited Warranty	136
----------------------------------	------------


IDENTIFICATION

1.1. Product Brand

The **SKOOT** is a remotely operated vehicle with magnetic wheels suitable for driving on ferrous material. Its primary purpose is to move inspection equipment over areas of structures, such as tanks or pipes, made from ferrous materials in industrial environments.

1.2. Manufacturer

Distributor:



Manufacturer:

Jireh Industries Ltd.
53158 Range Road 224
Ardrossan, Alberta, Canada
T8E 2K4
Phone: 780.922.4534
jireh.com

1.3. Compliance Declarations

1.3.1. ISED Emissions Compliance (Canada)

CAN ICES-003(A) / NMB-003(A)

This Class A digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe A est conforme à la norme NMB-003 du Canada.

1.3.2. FCC Suppliers Declaration of Conformity (United States)

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

RESPONSIBLE PARTY NAME:	Jireh Industries
ADDRESS:	2955 S Sam Houston Pkwy E Suite 300 Houston, Texas United States 77047
TELEPHONE:	832-564-0626

1.3.3. European Union CE Declarations

Jireh Industries hereby declares that the **SKOOT** product complies with the essential requirements and other relevant provisions of the following European Union directives:



- 2014/30/EU EMC Directive
- 2014/35/EU Low Voltage Directive
- 2012/19/EU Directive on Waste Electrical and Electronic Equipment
- 2011/65/EU Directive on Restriction of Hazardous Substances (RoHS).

PRODUCT SPECIFICATIONS

2.1. Base SKOOT System

This section outlines the product specifications of the base system. When the base system is used together with compatible components (*Chapter 2.2*) or child products (*Chapter 2.3*), the product specifications of the base system may be superseded. See (*see “Compatible Components” on page 12*) and (*see “Child Products” on page 17*)

2.1.1. Intended Use



WARNING! FALLING OBJECT HAZARD.

The **SKOOT** is intended for a specific use. Read and understand the intended and unintended use limits below. Using the **SKOOT** outside of its intended use is dangerous and could result in **SEVERE INJURY** or **DEATH**.

The **SKOOT**'s primary purpose is to perform inspections of ferrous assets such as pipes, vessels, or storage tanks by moving an inspection tool over a ferrous surface. It is intended for industrial use only.

2.1.1.1 Operating Limits

Category	Parameter	Specification
Inspection Surface	Maximum coating thickness:	
	Up-side-down orientation	Bare metal only
	Vertical orientation	0.5 mm (0.020 in)
	Horizontal, Right-side-up orientation	1 mm (0.040 in)
	Condition	Clean, free of excess rust, scale, debris (i.e. dirt, sand, etc.), ice, frost
	Minimum thickness	3 mm (0.120 in)
	Minimum ID, internal circumferential driving	686 mm (27 in)
	Minimum OD, external Circumferential driving	64 mm (2.5 in)
	Minimum OD, longitudinal driving	762 mm (30 in)
	Maximum surface temperature	50°C (122°F)

Category	Parameter	Specification
Scanner	Maximum umbilical length	30 m (100 ft)
	Maximum payload <i>(performance may vary with surface condition)</i>	9 kg (20 lb) <i>(Umbilical and attachments are considered payload)</i>
	Attachments	Restricted to those listed in compatible components or child products
	Orientation while driving at height >2 m (6 ft) on vertical surface	Umbilical strain relief to point downwards, or at worst, horizontal. It is not to point upwards
	Required radial clearance <i>(stick handle and backpack removed, front handle lowered, circumferential driving)</i>	102 mm (4 in) on outer diameters <200 mm (8 in) 112 mm (4.4 in) on outer diameters >200 mm (8 in)
Backpack	Maximum weight of mounted object	1.36 kg (3 lb)
	Condition of mounted object	Attached to crawler with lanyard or cables strong enough to prevent object from falling
		Smooth edges to prevent cutting of strap

2.1.1.2 Operating Environment

The SKOOT is for use in dry industrial environments having ambient temperatures shown below. It is **NOT** intended for use in explosive environments

Category	Parameter	Specification
Environment	Minimum ambient temperature	-20°C (-4°F)
	Maximum ambient temperature	50°C (122°F)

2.1.1.3 User

The SKOOT is intended to be used by persons who have read and understand the user manual. The intended user is to be a person without limitations in the physical abilities of the upper and lower limbs, sight, hearing, or anyone with a pacemaker or Implantable Cardioverter Defibrillator (ICD).

For operating at a height greater than 2 m (6 ft), the SKOOT is intended to be used by two people:

1. a person who is trained in rigging and fall protection and is able to effectively apply the same safety principles to the crawler, and
2. a person who is trained to operate the SKOOT

2.1.2. Unintended Use

The SKOOT is NOT intended for:

- ▶ use outside of its intended use
- ▶ unattended use
- ▶ lifting / lowering objects or people (*i.e. using the SKOOT as a crane / elevator*)
- ▶ driving into / over obstructions, excluding standard weld caps
- ▶ installation on a surface on which welding is actively occurring

In addition to the above points, for operating at a height greater than 2 m (6 ft), the crawler is NOT intended for:

- ▶ operation without a properly cordoned off no entry fall zone and/or proper tether system
- ▶ operating up-side-down
- ▶ operating while oriented such that the umbilical strain relief points upward (*front for the SKOOT is lower than the umbilical connection*).

2.1.3. Dimensions and Weight

Crawler height:	14.9 cm	5.9 in
Crawler width:	20.8 cm	8.2 in
Crawler depth:	21.8 cm	8.6 in
Crawler height (<i>handle down</i>):	11.2 cm	4.4 in
Crawler weight: *	7.3 kg	16 lb

* Configuration excluding case, attachments, umbilical, manipulation handle, power controller and handheld controller.

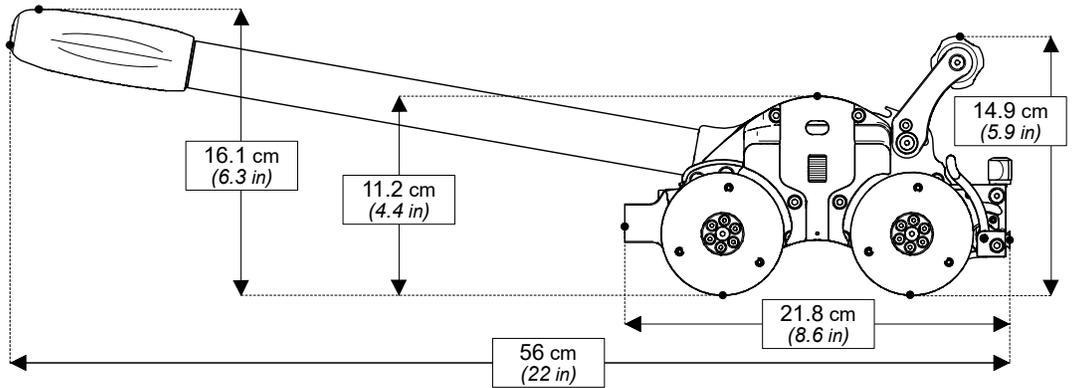


Fig. 1 - Crawler dimensions

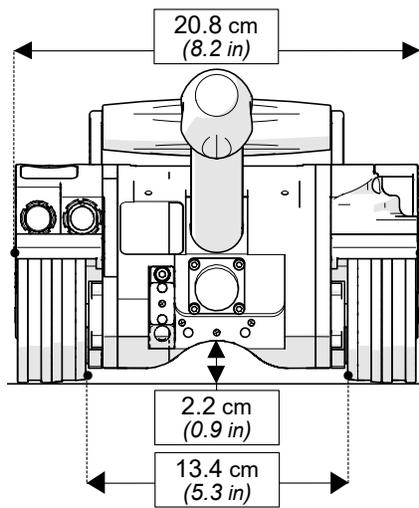


Fig. 2 - Width

2.1.4. Power Requirements



WARNING! A reliable power source must be used to power the crawler. Connections must be secured to prevent accidental disconnection. Power failure may cause the crawler to freewheel down when operating in a vertical orientation. Portable generator usage is not recommended unless accompanied by the use of an uninterruptible power controller.



WARNING! Proper grounding of the power controller is important for safe operation. When a generator is used to supply power to the system (*not recommended*), the generator must be properly grounded (*refer to generator manual*).



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.



CAUTION! Power must be supplied from an approved Jireh power source.

Power Requirements: 100-240VAC, 50/60Hz, 1.4 Amps

2.1.5. Environmental Sealing

Dust-tight, watertight (*not submersible*).

2.1.6. Performance Specifications

Category	Parameter	Specification
Crawler	Maximum speed	14.2 cm/sec (5.6 in/sec)
	Encoder resolution, drive motor	1354 counts/mm (34394 counts/in)

2.1.7. Encoder Interface Specifications

Output type: 4 channel quadrature 5VDC RS422 compatible.

Power: Power must be supplied to the interface.

5VDC +/-10% power limited to < 15w.

1	Enc B
2	Enc B'
3	Enc A
4	Enc A'
5	Aux Enc A'
6	Aux Enc A
7	Aux Enc B'
8	Aux Enc B
9	Enc +5V
10	Enc Com
H	Shield

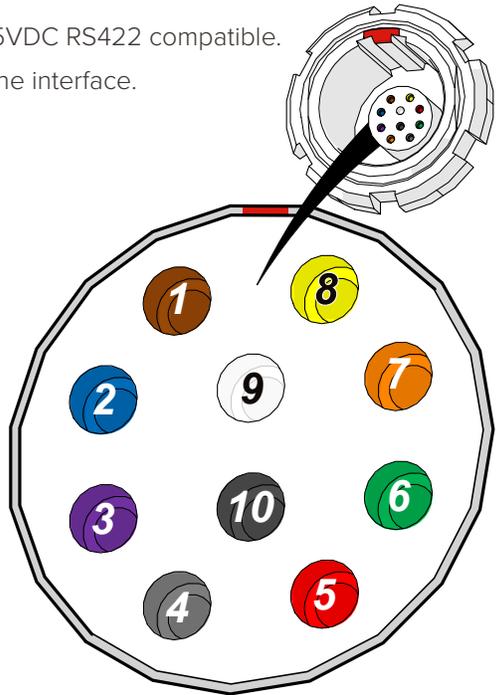


Fig. 3 - Jireh Industries pin out configuration

2.2. Compatible Components

The components listed in this section integrate with the base system to perform certain tasks. Their use may modify the product specifications (*i.e. intended use, power requirements, etc.*) from those of the base system. The specifications listed here supersede those of the base system. If no specifications are listed here, the specifications of the base system remain effective.

2.2.1. Low Profile Probe Holder Frame CXG004-

2.2.1.1 Intended Use

The Low Profile Probe Holder Frame is intended to be mounted in the SKOOT's swivel mount to provide mounting of multiple probe holders. Its use limits the SKOOT's operation to inspection surfaces that are either flat or driven on in the circumferential direction.

2.2.1.2 Operating Limits

Category	Parameter	Specification
Inspection Surface	Minimum OD, longitudinal driving	Not recommended
Maximum number of probe holders	Slip joint probe holders	4

2.2.2. Vertical Probe Holder Frame CXG007-

2.2.2.1 Intended Use

The Vertical Probe Holder Frame is intended to be mounted in the SKOOT's swivel mount to provide mounting of multiple probe holders. Its use limits the SKOOT's operation to inspection surfaces that are either flat or driven on in the circumferential direction.

2.2.2.2 Operating Limits

Category	Parameter	Specification
Inspection Surface	Minimum OD, longitudinal driving	Not recommended
Maximum number of probe holders	Vertical probe holders	6

2.2.3. Pivoting Probe Holder Frame CXG013-

The Pivoting Probe Holder Frame is intended to be mounted in the SKOOT's swivel mount to provide mounting of multiple probe holders. Its use limits the SKOOT's operation to the operating limits shown below.

2.2.3.1 Operating Limits

Category	Parameter	Specification
Maximum number of probe holders	Vertical probe holders	6

2.2.4. Frame Bar BG0038-

2.2.4.1 Intended Use

The Frame Bar is intended to be mounted in the SKOOT's swivel mount to provide mounting of multiple probe holders. Its use limits the SKOOT's operation to inspection surfaces that are either flat or driven on in the circumferential direction.

2.2.4.2 Operating Limits

Category	Parameter	Specification
Inspection Surface	Minimum OD, longitudinal driving	Not recommended
Maximum number of probe holders	Slip joint probe holders	2
	Vertical probe holders	2
	Heavy duty vertical probe holders	2

2.2.5. Slip Joint Probe Holder PHA012-

The Slip Joint Probe Holder is intended to provide a probe holding solution for probes and wedges with pivot button holes. It is useful for situations requiring lower profile. It is mounted in the dovetail groove of any probe holder frame or frame bar.

2.2.6. Vertical Probe Holder PHA015-

The Vertical Probe Holder is intended to provide a probe holding solution for probes and wedges with pivot button holes. It is mounted in the dovetail groove of any probe holder frame or frame bar.

2.2.7. Heavy Duty Vertical Probe Holder PHS043-

The Heavy Duty Vertical Probe Holder is intended to provide a probe holding solution for larger, heavier probes. It is mounted in the dovetail groove of any probe holder frame or frame bar.

2.2.8. Corrosion Thickness Probe Holder PHS046- / PHS056-

The Corrosion Thickness Probe Holder is intended to provide a probe holding solution for specific probes or wedges that do not have pivot button holes. It is mounted in the dovetail groove of any probe holder frame or frame bar.

2.2.9. HydroFORM Cart with Wheels PHS044

The HydroFORM Cart with Wheels is intended to provide a solution for holding the Olympus HydroFORM probe. It is used in conjunction with the heavy duty vertical probe holder.

2.2.10. Preamp Bracket CES029-

2.2.10.1 Intended Use

The Preamp Bracket is intended to mount objects such as preamps, splitters, etc. on a rack or dovetail bar that is mounted to the SKOOT crawler. The mounted object is attached to the SKOOT with a lanyard or probe cables strong enough to prevent the object from falling, should the straps or screws that hold it to the bracket fail. Also, if the object is mounted with straps, it is to have smooth edges so as not to cut the straps.

2.2.10.2 Operating Limits

Category	Parameter	Specification
Preamp Bracket	Maximum weight of mounted object	1.36 kg (3 lb)
Scanner	Required radial clearance (<i>handles removed circumferential driving</i>)	Dependent on object mounted on Preamp Bracket

2.2.11. Battery Powered Optical Guide CXS080

2.2.11.1 Intended Use

The Battery Powered Optical Guide is intended to provide a point of reference useful for guiding the SKOOT along a given path (*i.e. a weld cap*). It is intended to be mounted in the dovetail groove of any probe holder frame or frame bar.

2.2.11.2 Operating Environment

Category	Parameter	Specification
Scanner	Required radial clearance	Dependent on mounted orientation of Optical Guide

2.2.11.3 Power Requirements

Power requirements: 1 AA battery

2.2.11.4 Environmental Sealing

IP64

2.2.12. Medium Temperature Add-On Kit CXG031-

2.2.12.1 Intended Use

The Medium Temperature Add-On Kit allows the SKOOT to operate on inspection surfaces that are hotter.

2.2.12.2 Operating Limits

Category	Parameter	Specification
Inspection surface	Maximum surface temperature	150°C (302°F)

2.2.13. Encoder Adapter UMA010-

2.2.13.1 Intended Use

The Adapter Cable adapts a scanner's existing encoder cable connector to a different instrument's encoder input.

2.3. Child Products

The products listed in this section integrate with the base system to perform certain tasks. Their use may modify the product specifications (*i.e. intended use, power requirements, etc.*) from those of the base system. These products have a user manual of their own, and shall be referred to for their product specifications as well as how their use modifies the product specifications of the base system.

2.3.1. Motorized Couplant Pump CMA015

The Motorized Couplant Pump is a powered pumping unit used to supply couplant fluid to scanning equipment.

2.3.2. Motorized Raster Arm CWG002-

Available in various lengths, the Motorized Raster Arm can carry many different probes for various types of corrosion scans. The Motorized Raster Arm is intended to be mounted in the SKOOT's swivel mount.

2.3.3. Optical Guide CXG035


The Optical Guide mount's to any dovetail attached to a motorized crawler. The Optical Guide provides a green colour, point of reference for guiding scanners along a given path (*i.e. a weld*).

DEFINITIONS

3.1. Definition of Symbols



Instructions to 'look here' or to 'see this part'.



Denotes movement. Instructing user to carry out action in a specified direction.



Indicates alignment axis.



Alerts user that view has changed to a reverse angle.

3.2. Definitions of Terms

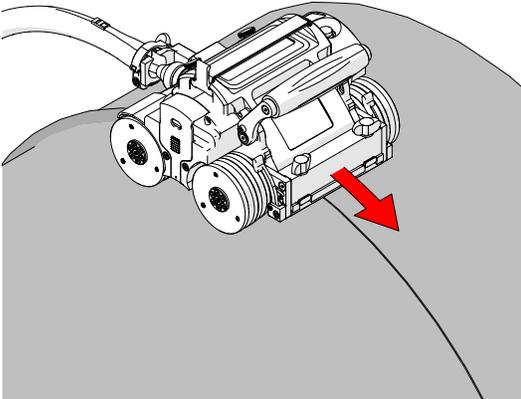


Fig. 4 - Circumferential scanning

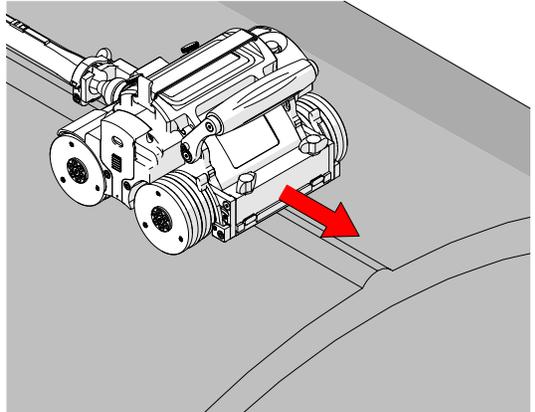


Fig. 5 - Longitudinal scanning

Circumferential

Direction of scan travel is around the circumference of the pipe/tube (Fig. 4).

Longitudinal

Direction of scan travel is lengthwise of the pipe/tube (Fig. 5).

3.3. Safety Symbols

The following safety symbols might appear on the product and in this document. Read and understand their meaning below:

	General warning symbol	This symbol is used to alert the user to potential hazards. All safety messages that follow this symbol shall be obeyed to avoid possible harm or material damage.
	Shock hazard caution symbol	This symbol is used to alert the user to potential electric shock hazards. All safety messages that follow this symbol shall be obeyed to avoid possible harm.
	Laser warning symbol	This symbol is used to alert the user to potential laser hazards. All safety messages that follow this symbol shall be obeyed to avoid possible harm or material damage.

3.4. Safety Signal Words

The following safety signal words might appear in this document. Read and understand their meaning below:

DANGER!

The DANGER signal word indicates an imminently hazardous situation. It calls attention to a procedure, practice, or the like that if not correctly performed or adhered to will result in death or serious personal injury. Do not proceed beyond a DANGER signal word until the indicated conditions are fully understood and met.

WARNING!

The WARNING signal word indicates a potentially hazardous situation. It calls attention to a procedure, practice, or the like that if not correctly performed or adhered to could result in death or serious personal injury. Do not proceed beyond a WARNING signal word until the indicated conditions are fully understood and met.

CAUTION!

The CAUTION signal word indicates a potentially hazardous situation. It calls attention to a procedure, practice, or the like that if not correctly performed or adhered to may result in minor or moderate personal injury, material damage, particularly to the product, destruction of part or all of the product, or loss of data. Do not proceed beyond a CAUTION signal word until the indicated conditions are fully understood and met.

SYSTEM COMPONENTS

4.1. Component Identification

4.1.1. Base System




Fig. 6 - SK00T (crawler)
DNA004




Fig. 7 - Backpack
DNS008

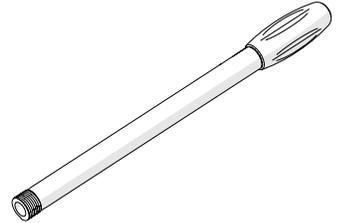


Fig. 8 - Manipulation handle
DNS006




Fig. 9 - Handheld controller
CXA008

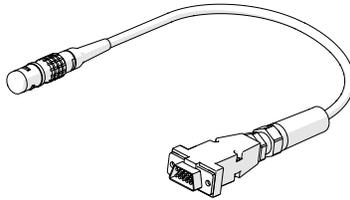


Fig. 10 - Encoder cable
UMA025-

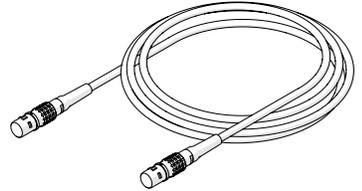


Fig. 11 - Auxiliary cable
UMA017-

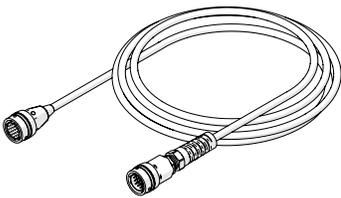


Fig. 12 - Umbilical
UMA022-

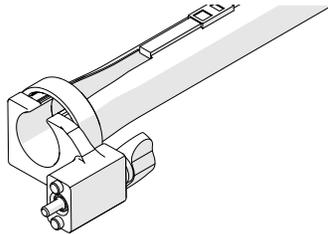


Fig. 13 - Cable management
CXS046-

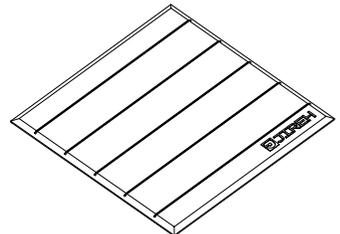


Fig. 14 - Installation/removal mat
AAS061




Fig. 15 - Battery powered optical guide
CXS080

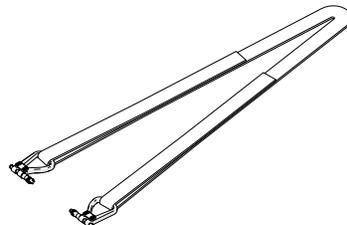


Fig. 16 - Lifting sling
EA243




Fig. 17 - Power controller
DNA006-

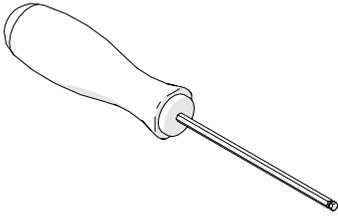


Fig. 18 - 3 mm hex driver
EA414

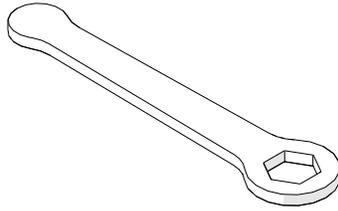


Fig. 19 - 3/8 in wrench
EA470

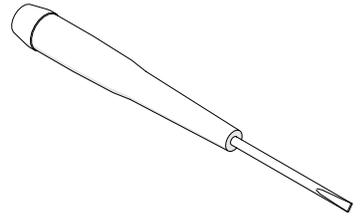


Fig. 20 - 3 mm flat driver
EA480




Fig. 21 - SK00T crawler case
DNA010




Fig. 22 - Umbilical / probe holder frame case
CXA023




Fig. 23 - Umbilical case
EA421




Fig. 24 - Motorized pump / umbilical case
CMA016

4.1.2. Compatible Components

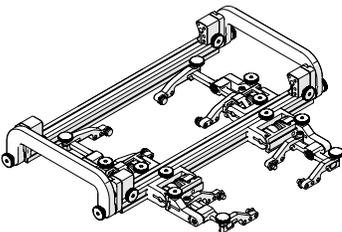


Fig. 25 - Low profile probe holder frame
CXG004-

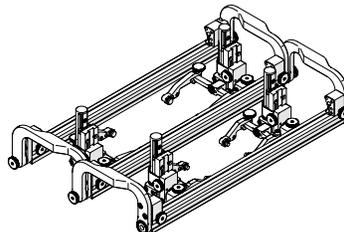


Fig. 26 - Vertical probe holder
CXG007-

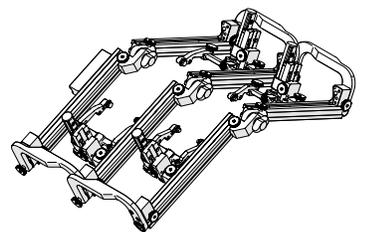


Fig. 27 - Pivoting probe holder frame
CXG013-

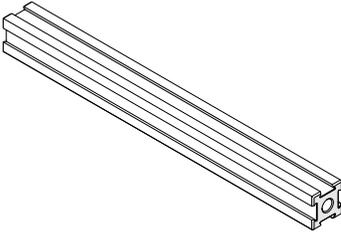


Fig. 28 - Frame bar
BG0038-




Fig. 29 - Slip joint probe holder
PHA012-




Fig. 30 - Vertical probe holder
PHA015-




Fig. 31 - Heavy duty vertical probe holder
PHS043-




Fig. 32 - Corrosion thickness probe holder
PHS046-

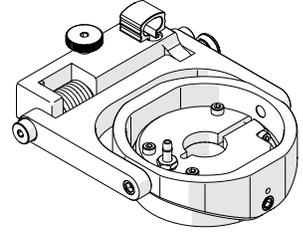


Fig. 33 - Corrosion thickness probe holder
PHS056-

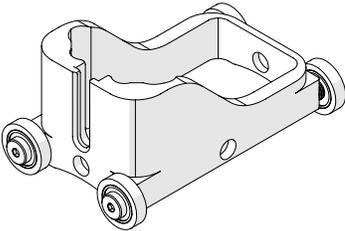


Fig. 34 - HydroFORM cart
PHS044




Fig. 35 - Pre-amp bracket
CES029-




Fig. 36 - Battery powered optical guide
CXs080

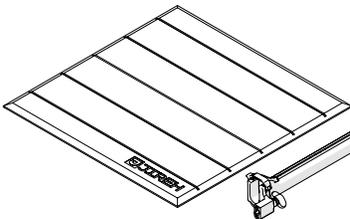


Fig. 37 - Automated crawler medium
temperature add-on kit
CXG031-

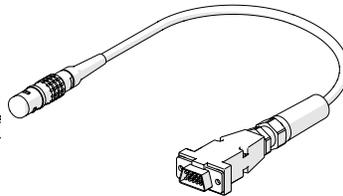


Fig. 38 - Encoder adapter
UMA010-

4.1.3. Child Products

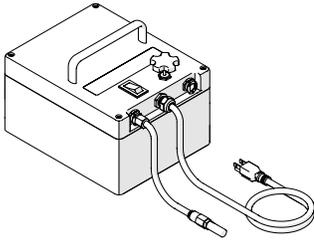


Fig. 39 - Motorized Couplant Pump
CMA015

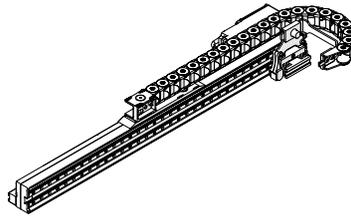


Fig. 40 - Motorized raster arm
CWG002-

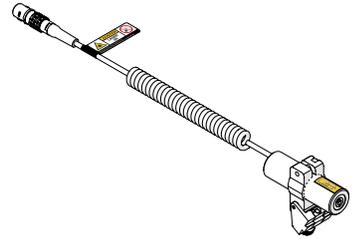


Fig. 41 - Optical Guide
CXG035

4.2. Tools

4.2.1. Included Tools

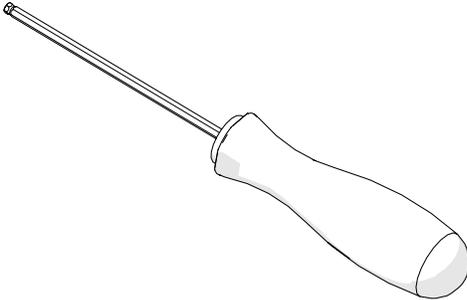


Fig. 42 - 3 mm hex driver

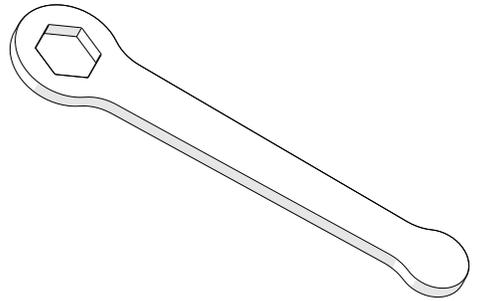


Fig. 43 - 3/8 in wrench

The included 3 mm hex driver (Fig. 42) is suitable for typical **SKOOT** and probe holder adjustments.

A 3/8 in wrench (Fig. 43) is provided to remove and install probe holder buttons.

The included 3 mm flat driver (Fig. 44) is useful for releasing the flaps of the raster arm's cable tray.

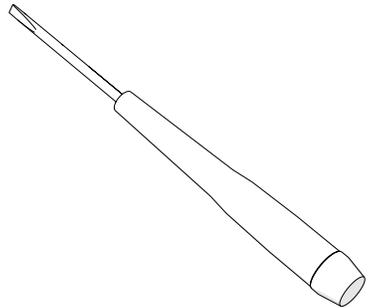


Fig. 44 - 3 mm flat driver

4.2.2. Optional tools

Some specialized adjustments require tools that are not included with this kit.




Fig. 45 - 1.5 mm hex wrench




Fig. 46 - 2 mm hex wrench

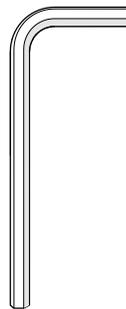


Fig. 47 - 2.5 mm hex wrench

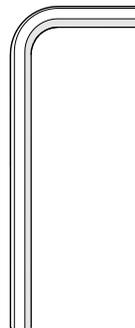


Fig. 48 - 3 mm hex wrench

4.3. Base System Components

4.3.1. Crawler

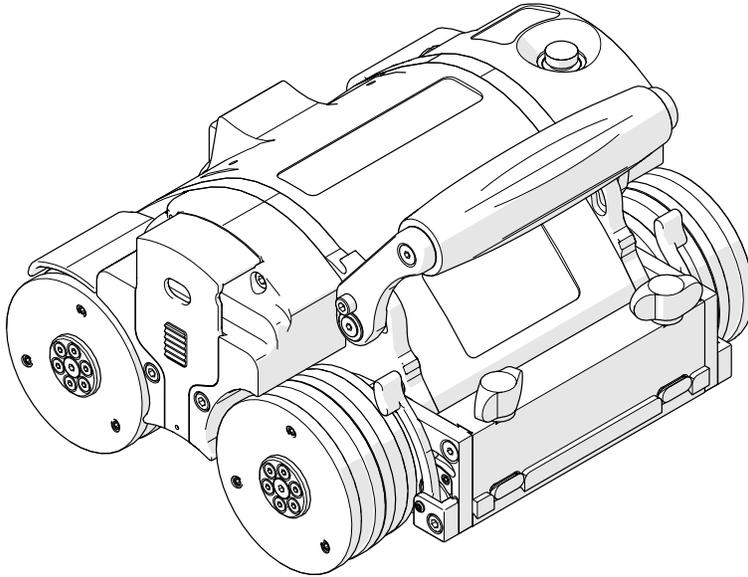


Fig. 49 - Crawler

The crawler includes the motor encoder, umbilical connections and accessory mounting point.

4.3.1.1 Emergency Off Button

The red button located on the top left of the crawler provides an emergency off button to the entire system. When pressed, all power to the **SKOOT** system will disengage.

NOTE: Terminating system power may cause the crawler to freewheel down when operating in a vertical orientation.




Fig. 50 - Emergency off

4.3.2. Power Controller



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.



WARNING! There are no user serviceable components inside the power controller. Dangerous voltages can be present inside the case. Do **NOT** open. Return to manufacturer for repair.

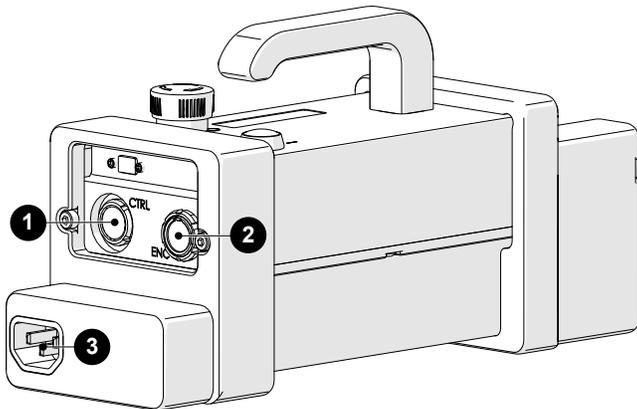


Fig. 51 - Power controller

The **SKOOT** power controller converts power from a 100-240 VAC, 50/60Hz, 1.4A power source to 36VDC, 2.65A. A start/stop safety circuit and physical **ON** and **OFF** push-buttons are integrated into the supply.

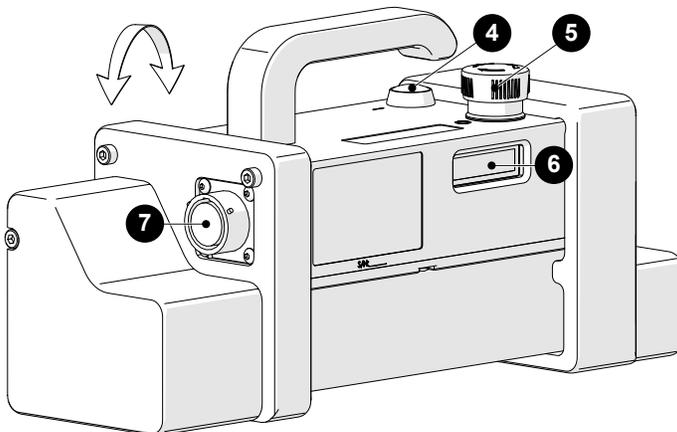


Fig. 52 - Power controller

1	CTRL socket	Connection for the auxiliary cable
2	ENC socket	Connection for the encoder cable
3	Power connection	Connect plug from a properly grounded source. Use IEC320 cord approved for AC supply
4	Power button	Activate system power by pressing (and releasing) the green button.
5	Stop button	The red stop button latches down when pressed, this stop button shuts down the system. Twist the stop button clockwise to return to the released position. This must be done before power can be activated.
6	Status LCD	Displays the power controller's status.
7	Umbilical connection	Connection for the umbilical.

In the event of a break in the stop circuit (*the stop circuit runs through the power controller cable, umbilical and the crawler's emergency stop button*) power will shut off.

NOTE: Before use, always inspect the power cable and plug for damage. The power controller should not be used if visible damage is present. Use of damaged components may be a safety hazard.

4.3.2.1 AC/DC Power Supply

The power connection **3** of the power controller is used to connect the power controller to a suitable 90-270VAC, 45-65Hz grounded power source capable of supplying a minimum of 5 amps.

The safety of the power controller relies on the provision of a proper ground connection.

In environments with moisture present, a GFCI (Ground Fault Circuit Interrupter) must be used to ensure operator safety.

NOTE: Some generators or DC-AC inverters may introduce significant levels of noise to the system. This may degrade overall system performance or reduce the system life expectancy. Use of generators or DC-AC inverters is not recommended and are used at the operator's risk.

4.3.3. Handheld Controller



CAUTION! DO NOT DISCONNECT UNDER

LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.

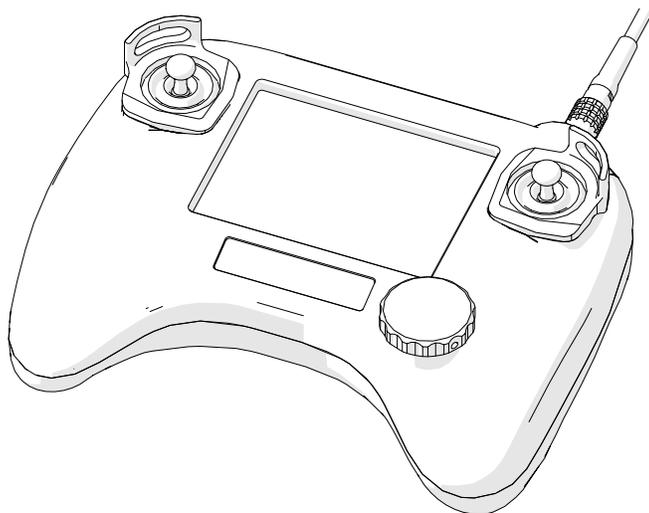


Fig. 53 - Handheld controller

The handheld controller is used to manipulate a scanner installed on an inspection surface. User settings and scan information are edited using the handheld controller. The handheld controller is connected to the power controller with the auxiliary cable.

The handheld controller contains the complete system program and must be connected for the system to operate. When a software upgrade is necessary, the handheld controller is the only component required.

The handheld controller is not watertight and is not intended to be used in extremely wet environments. The handheld controller utilizes a resistive touch screen, care should be taken to not use sharp or gritty objects on the screen as the touch membrane can scratch. If the screen is damaged, all programmed functions can still be accessed using the click wheel.

NOTE: Do **NOT** connect the handheld controller while system activated.

4.3.4. Auxiliary Cable

The auxiliary cable connects the handheld controller to the power controller. 36VDC and network signals are used in the cable.

Both auxiliary cable connectors are identical and interchangeable. The cable may be plugged into the 4-pin receptacle on the power controller or the crawler's umbilical.

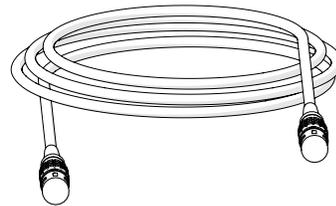


Fig. 54 - Auxiliary cable

NOTE: Inspect the cable and connectors for damage before use. When any damage is evident, the cable must **NOT** be utilized. Use of a damaged cable may be a safety hazard and could also put other system components at risk.

4.3.5. Encoder Cable

The encoder cable connects the **SKOOT** system to the user's instrument. This cable allows transmission of two-axis position signals from the **SKOOT** to the instrument. The encoder cable also provides 5VDC from the user's instrument to the encoder isolation circuitry.

Various encoder styles are available for various instruments.

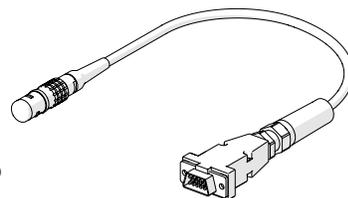


Fig. 55 - Encoder cable

NOTE: Inspect the cable and connectors for damage before use. When damage is evident, the cable must **NOT** be used.

4.3.6. Installation/Removal Mat



WARNING! MAGNETIC MATERIAL. The installation/removal mat contains magnetic material. Those with pacemakers or ICD's must stay at least 10 cm (4 in) away.



The installation/removal mat is used for installation and removal of motorized magnetic-wheeled scanners from the inspection surface. A motorized scanner can drive on/off the mat, while the integrated magnets in the mat hold it firmly in place on the inspection surface. The scanner installation mat can be used on both round and flat surfaces.

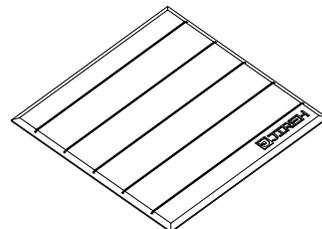


Fig. 56 - Installation/removal mat

4.3.7. Lifting Sling

The lifting sling attaches to the crawler to provide an attachment point for tethers. When operating a **SKOOT** at a height greater than 2 m (6 ft), the crawler **MUST** be tethered with a proper tether system to prevent the crawler from falling (see "Preparation for Safe Use" on page 35).

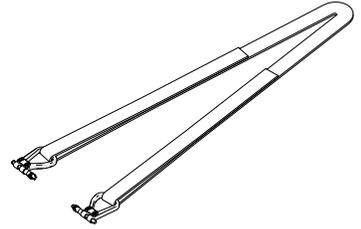


Fig. 57 - Lifting sling

4.3.8. Irrigation Kit

The irrigation kit provides a variety of hoses, fittings, connectors and splitters commonly used during non-destructive inspection.

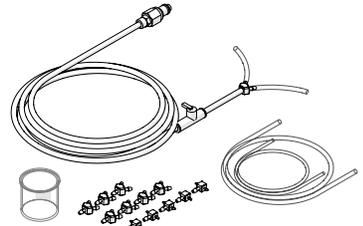


Fig. 58 - Irrigation kit

4.3.9. Cable Management

The cable management provides a means of protecting and organizing cables, tubes and hoses.

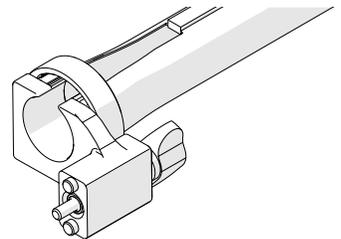


Fig. 59 - Cable management

4.3.10. Tools

Several tools are included for various scanner and accessory adjustment. (see "Tools" on page 24 for additional details)

4.3.11. Cases

Depending on the configuration selected at the time of purchase. This will determine the types and amount of cases included with the system.

4.4. Compatible Components

4.4.1. Low Profile Probe Holder Frame

The low profile probe holder frame carries up to four probes during limited access, circumferential weld inspection. Removal of the **SKOOT** handles and the use of the low profile probe holder frame allows inspection when radial clearance is limited.

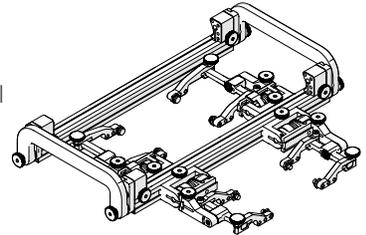


Fig. 60 - Low profile probe holder frame

4.4.2. Vertical Probe Holder Frame

The vertical probe holder frame carries up to six probes during circumferential weld inspection. Available in a myriad of configurations and lengths, the vertical probe holder frame attaches to the front of the **SKOOT** crawler.

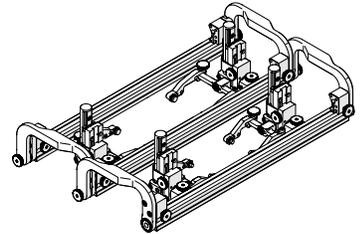


Fig. 61 - Vertical probe holder frame

4.4.3. Pivoting Probe Holder Frame

The pivoting probe holder frame carries up to six probes during longitudinal weld inspection. Available in a myriad of configurations and lengths, the pivoting probe holder frame may also be used for circumferential weld inspection.

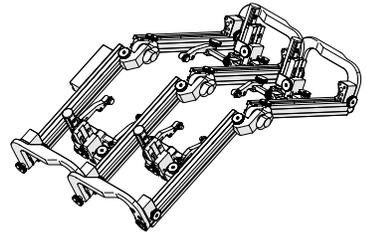


Fig. 62 - Pivoting probe holder frame

4.4.4. Frame Bar

Frame bars use dovetail grooves into which probe holders and accessories may be attached. Available in various lengths.

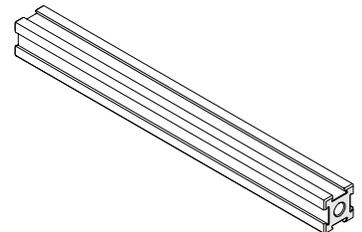


Fig. 63 - Frame bar

4.4.5. Slip Joint Probe Holder

The slip joint probe holder is generally used during limited access inspection. The low profile design requires minimal radial clearance. The slip joint probe holder is designed to carry many different types of probes and wedges, it is available with various types of yokes, arms and pivot buttons.




Fig. 64 - Slip joint probe holder

4.4.6. Vertical Probe Holder

The vertical probe holder is designed to carry many different types of probes and wedges. Available with various types of yokes, arms and pivot buttons. The vertical probe holder features several different adjustment options for each unique probe/wedge setup.




Fig. 65 - Vertical probe holder

4.4.7. Heavy Duty Vertical Probe Holder

The heavy duty vertical probe holder is designed to carry larger probes. Available with various arm, yoke and pivot buttons, the heavy duty vertical probe holder exerts more down force on a large footprint probe/wedge.




Fig. 66 - Heavy duty vertical probe holder

4.4.8. Corrosion Thickness Probe Holder

The corrosion thickness probe holder carries various probes for the purpose of corrosion inspection and is available with either a flat or curved wear plate.




Fig. 67 - Corrosion thickness probe holder

4.4.9. HydroFORM Cart

The HydroFORM Cart carries an Olympus HydroFORM™ probe. The HydroFORM cart is designed to be used in conjunction with the heavy duty vertical probe holder.

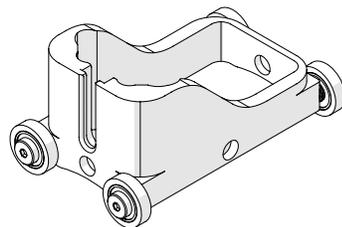


Fig. 68 - HydroFORM cart

4.4.10. Preamp Bracket

The preamp mounts to any dovetail groove. It is compatible with more standard preamps.




Fig. 69 - Preamp bracket

4.4.11. Battery Powered Optical Guide

The battery powered optical guide provides a red colour point of reference useful for guiding scanners along a given path (*i.e. a weld*).




Fig. 70 - Battery powered optical guide

4.4.12. Automated Crawler Medium Temperature Add-On Kit

The automated crawler medium temperature add-on kit enables a **SKOOT** crawler to operate on an inspection surface with a temperature up to 150°C (302°F).

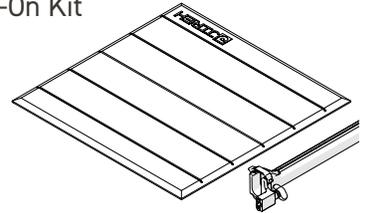


Fig. 71 - Automated crawler medium temperature add-on kit

4.4.13. Encoder Adapter

The encoder adapter changes the scanner's built in encoder connector style.

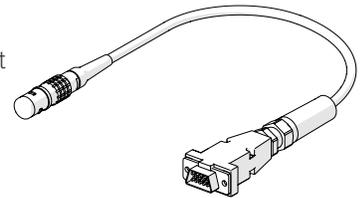


Fig. 72 - Encoder adapter

4.5. Child Products

4.5.1. Motorized Couplant Pump

The motorized couplant pump is a powered pumping unit used for supplying couplant fluid to the scanning surface.

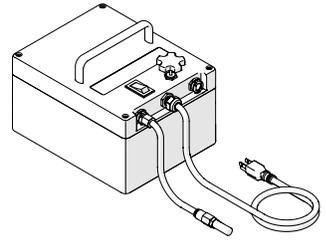


Fig. 73 - Motorized couplant pump

4.5.2. Motorized Raster Arm

The motorized raster arm is available in various lengths and offers programmable speed and travel settings.

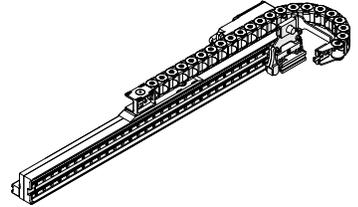


Fig. 74 - Motorized raster arm

4.5.3. Optical Guide

The optical guide mounts to any dovetail and provides a green colour point of reference useful for guiding scanners along a given path (*i.e. a weld*).

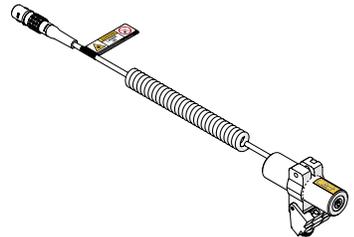


Fig. 75 - Optical guide

PREPARATION FOR USE

5.1. Preparation for Transportation



CAUTION! PINCH / CRUSH HAZARD. Be careful when passing the **SKOOT** crawler through narrow ferrous (*magnetic*) openings, such as man-holes. The magnetic drive wheels can cause bodily harm if allowed to slam onto the walls of the opening.

5.2. Preparation for Safe Use

5.2.1. No Entry Fall Zone



WARNING! FALLING OBJECT HAZARD. The area below a crawler must be kept clear at all times. A clearly marked **NO ENTRY FALL ZONE** must be cordoned off directly below the area of crawler operation.

The area below a crawler must be kept clear at all times. A clearly marked **NO ENTRY FALL ZONE** must be cordoned off directly below the area of crawler operation, according to the dimensions shown in (Fig. 76).

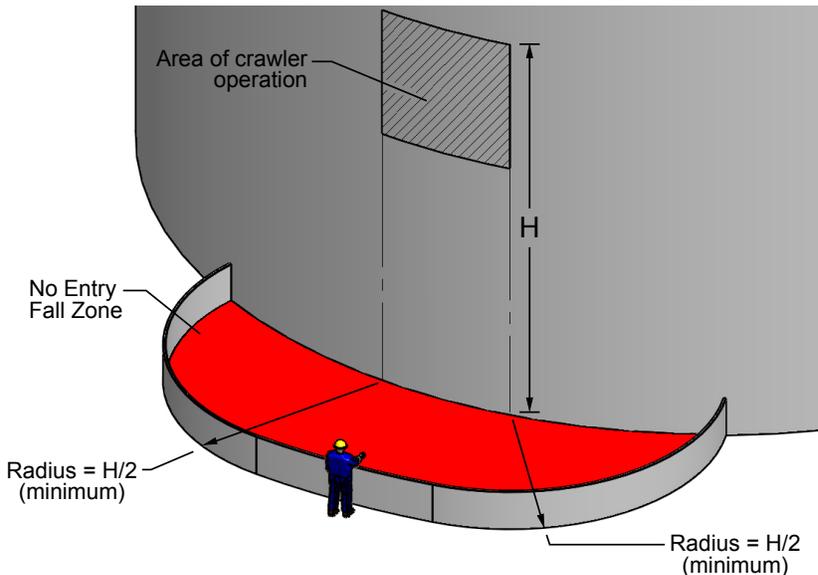


Fig. 76 - No entry fall zone

Example: If inspecting a tank that is 6 m (20 ft) tall, the No Entry Fall Zone radii must be no smaller than 3 m (10 ft) from the area below the area of crawler operation.

5.2.2. Tether Requirements and Attachment



WARNING! FALLING OBJECT HAZARD.

Failure to comply with the warnings, instructions, and specifications in this manual could result in **SEVERE INJURY** or **DEATH**.

WARNING! Do **NOT** operate or place crawler on a surface higher than 2 m (6 ft) without a proper tether held taut at all times.

WARNING! Hook the tether hook to the provided lifting sling **BEFORE** placing the crawler on the surface to be inspected (*e.g. tank*).

IMPORTANT: Tether hook must have a safety latch to prevent accidental disconnection.

When used at a height greater than 2 m (6 ft), the **SKOOT** crawler **MUST** be tethered with a proper tether system to prevent the crawler from falling. The tether system must:

- ▶ be capable of safely suspending the crawler from above in case the crawler detaches from the inspection surface;
- ▶ have sufficient capacity to catch and hold a 70 kg (150 lb) load;
- ▶ include a mechanism (*i.e. self retracting inertia reel fall arrester*) or person to continuously take up slack in the tether as the crawler moves;
- ▶ include a lifting hook with a safety latch to prevent accidental disconnection. The hook must be free of sharp edges that may cut or abrade the provided lifting sling.

Before placing the crawler on the surface to be inspected (*e.g. tank*), attach the provided lifting sling to the **SKOOT** and then hook the tether hook to the lifting sling.



CAUTION! The overhead attachment point for the tether must be located as close as possible to a location directly above the crawler to minimize dangerous swinging of the crawler should it detach from the inspection surface.

5.2.3. Lifting Sling Setup



IMPORTANT! Carefully inspect the lifting sling for damage prior to each use. Ensure the tether hook does not have sharp edges that may cut the lifting sling.

Secure the lifting sling to the **SKOOT** as illustrated here:

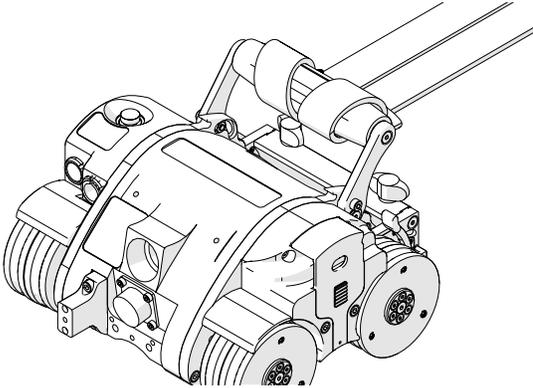


Fig. 77 - Attach the lifting sling with a choker hold

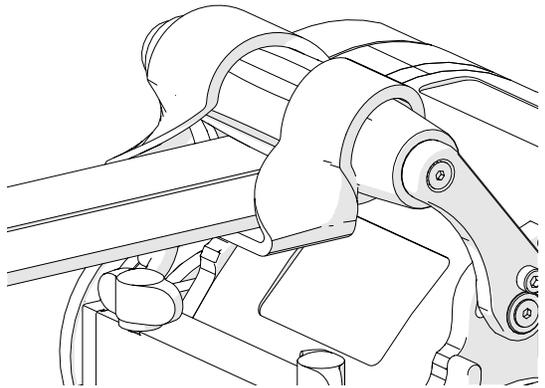


Fig. 78 - Attach the lifting sling with a choker hold

1. Wrap the supplied lifting sling around the handle of the **SKOOT** using a choker hold knot (Fig. 77) and (Fig. 78).
2. Ensure the lifting sling is attached correctly to the **SKOOT** and inspect the lifting sling for any damage prior to use.

5.3. Preparation of Inspection Surface



WARNING! FALLING OBJECT HAZARD.

The inspection surface must adhere to the conditions outlined in sections “Intended Use” on page 5 and “Operating Environment” on page 7 of this manual.

- ▶ Remove build-up of scale, and other debris (*i.e. dirt, ice*) from surface on which the crawler is to drive. Excessive build-up will cause the wheels to lose magnetic attraction which may lead to wheel slippage or crawler detachment.
- ▶ Ensure that no obstructions (*other than standard butt welds*) or voids are in the drive path. Obstructions and voids could cause the crawler to fall if driven into or over.
- ▶ Ensure that there are no patches of non-ferrous material in the drive path of the crawler. If the crawler drives over a non-ferrous patch, it will lose magnetic attraction and will cause the crawler to fall.

5.4. System Connectivity

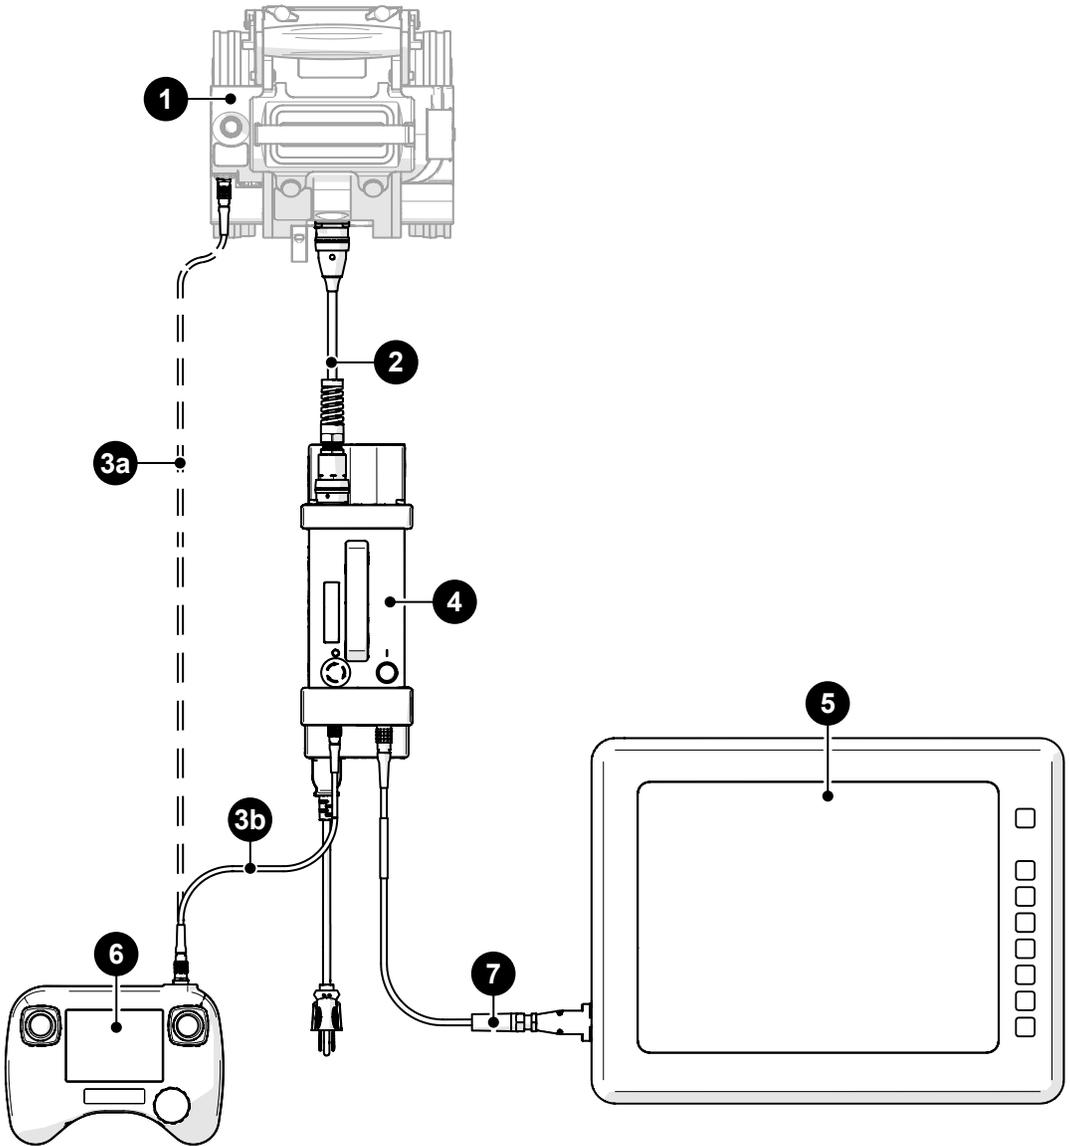


Fig. 79 - Standard crawler configuration

BOM ID	Description
1	Crawler
2	Umbilical
3a	Auxiliary cable (<i>alternate</i>)
3b	Auxiliary cable
4	Power controller
5	User instrument
6	Handheld controller
7	Encoder cable

To configure the **SKOOT** system for scanning, follow these steps:



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.

1. Connect the **4** power controller to the **1** crawler using the **2** umbilical.
2. Connect the **6** handheld controller to the **4** power controller using the **3b** auxiliary cable.

NOTE: The **6** handheld controller may also be connected directly to the **1** crawler using the **3a** auxiliary cable.

3. Connect the **5** user's instrument to the **4** power controller using the **7** encoder cable.
4. (see "Configurations" on page 40) to setup a particular component.

5.5. Configurations

5.5.1. Crawler with Multiple Probe Holders

5.5.1.1 Vertical Probe Holder Frame

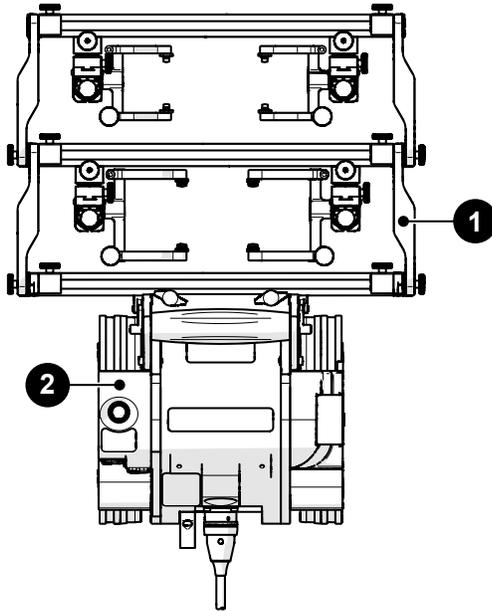


Fig. 80 - Probe holder frame configuration

BOM ID	Description
1	Vertical probe holder frame
2	Crawler

To configure the **SKOOT** system for scanning using a vertical probe holder frame, follow these steps (see “Vertical Probe Holder Frame - Flat or Circumferential Only” on page 76):



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.



1. Attach a configured **1** vertical probe holder frame to the **2** crawler.

5.5.1.2 Low Profile Probe Holder Frame

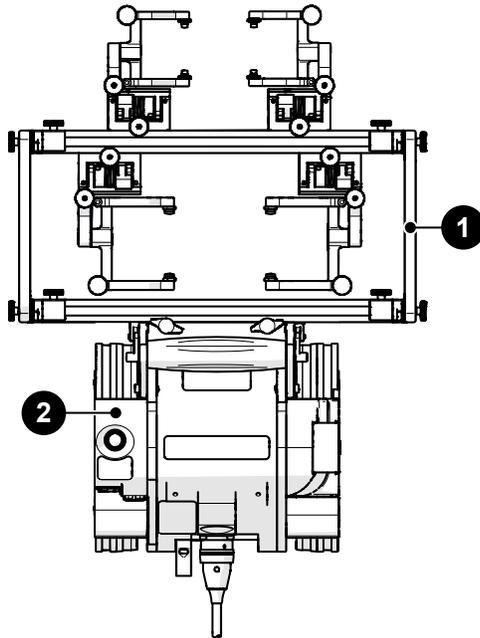


Fig. 81 - Low profile probe holder frame configuration

BOM ID	Description
1	Low profile probe holder frame
2	Crawler

To configure the **SKOOT** system for scanning using a low profile probe holder frame, follow these steps (see “*Low Profile Probe Holder Frame - Flat or Circumferential Only*” on page 72):



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.



1. Attach a configured **1** low profile probe holder frame to the **2** crawler.

5.5.1.3 Pivoting Probe Holder Frame

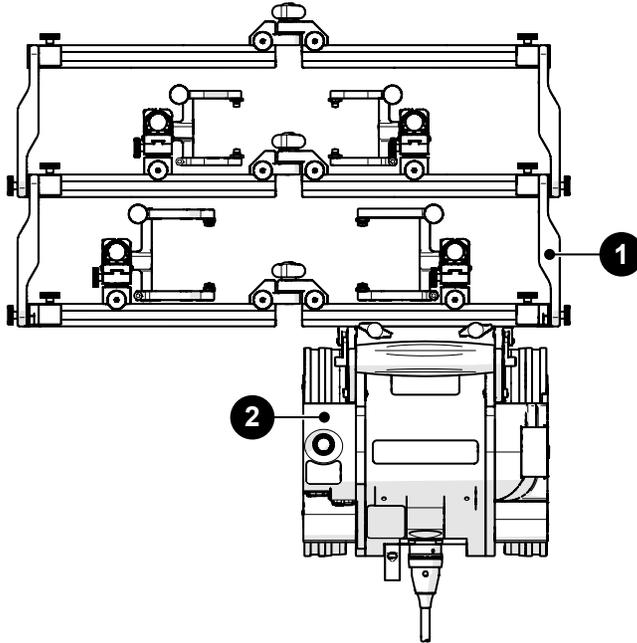


Fig. 82 - Pivoting probe holder frame configuration

BOM ID	Description
1	Pivoting probe holder frame
2	Crawler

To configure the **SKOOT** system for scanning using a pivoting probe holder frame, follow these steps (see “Pivoting Probe Holder Frame” on page 80):



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.

1. Attach a configured **1** pivoting probe holder frame to the **2** crawler.

5.5.1.4 Pivoting Probe Holder Frame

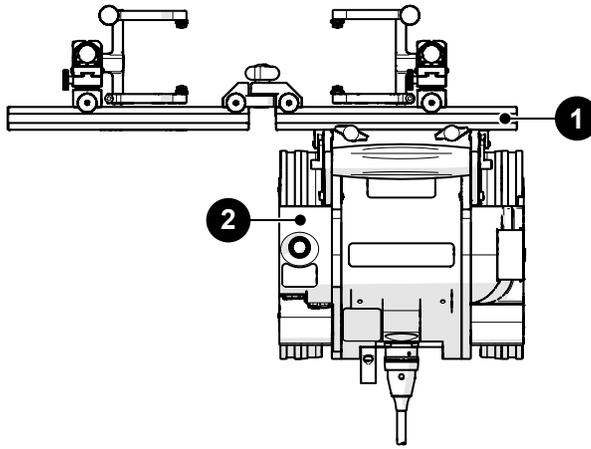


Fig. 83 - Pivoting probe holder frame configured for flange scanning

BOM ID	Description
1	Flange probe holder frame
2	Crawler

To configure the **SKOOT** system for scanning using a pivoting probe holder frame configured for flange scanning, follow these steps (see “*Pivoting Probe Holder Frame - Flange Scanning*” on page 84):



CAUTION! DO NOT DISCONNECT UNDER LOAD. Shut off power before connection or disconnecting. Permanent damage to electronics could occur.



1. Attach a configured **1** flange probe holder frame to the **2** crawler.

5.6. Crawler

5.6.1. Swivel Mount

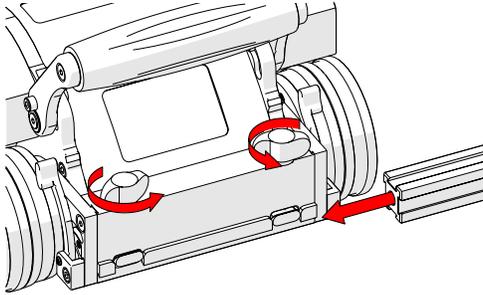


Fig. 84 - Frame bar installation

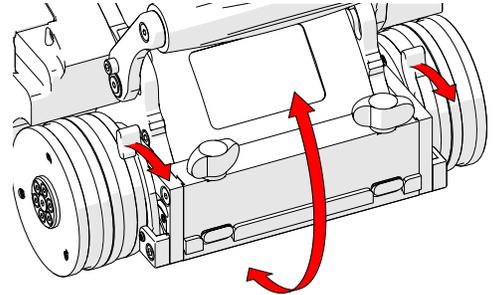


Fig. 85 - Swivel mount angle

Located at the front of the crawler, the swivel mount is used to connect scanning accessories such as a raster arm module, probe frame system or corrosion thickness probe holder.

Rotate the two black wing knobs (*Fig. 84*) to loosen the dovetail jaws. Slide the accessory's frame bar along the dovetail jaws. Rotate the two black wing knobs to clamp the frame system/raster arm in place.

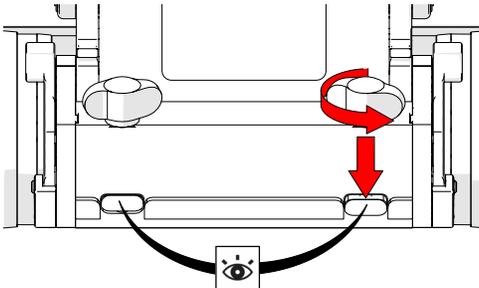


Fig. 86 - Align dovetail jaws

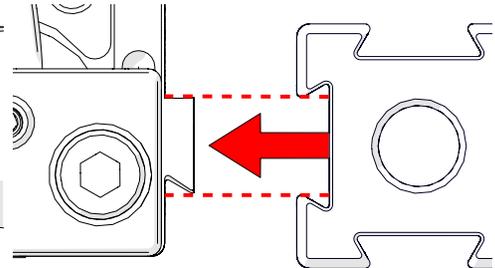


Fig. 87 - Mount frame bar

Alternatively, accessories can also be mounted straight to the swivel mount. Rotate the black wing knobs aligning the dovetail jaws with the mount's grooves (*Fig. 86*). Press the frame bar or accessory to the swivel mount (*Fig. 87*) and tighten the black wing knobs.

The front mount utilizes two levers (*Fig. 85*) to lock the front mount at the desired angle.

The etched line (Fig. 88) near the base of the swivel mount can be used to align the front swivel mount to a horizontal position.

NOTE: The front mount must be horizontal when using the pivoting probe holder frame to scan longitudinally on piping.

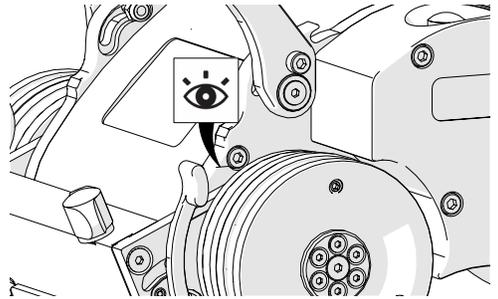


Fig. 88 - Return mount to horizontal position

5.6.2. Umbilical



WARNING! FALLING OBJECT HAZARD. or operating at heights greater than 2 m (6 ft), ensure the umbilical strain relief never points upwards as shown in (Fig. 92). The crawler could fall. **SEVERE INJURY** or **DEATH** could result.

To mount the umbilical to the crawler, follow these steps:

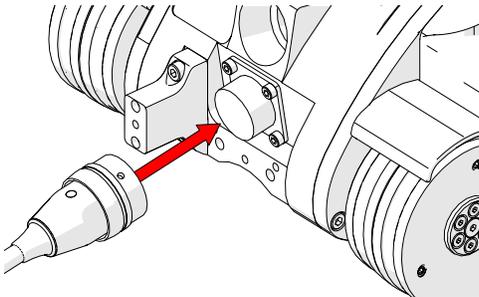


Fig. 89 - Connect to umbilical

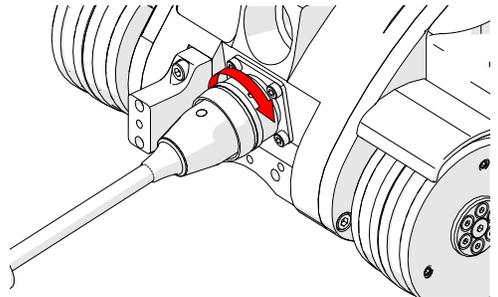


Fig. 90 - Align with crawler's umbilical mount

1. Align the pins of the umbilical to the connector at the rear of the **SKOOT** (Fig. 89).
2. Twist the umbilical's sleeve clockwise locking the umbilical in place (Fig. 90).

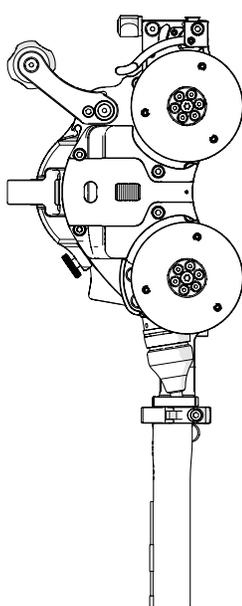


Fig. 91 - Correct umbilical use

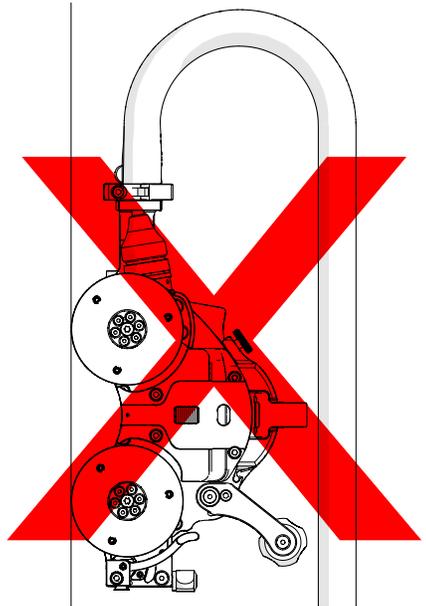


Fig. 92 - Incorrect umbilical use

3. Ensure the umbilical strain relief never points downwards during operation (Fig. 92).

5.6.3. Handle

The handle can be lowered to achieve low profile scanning.

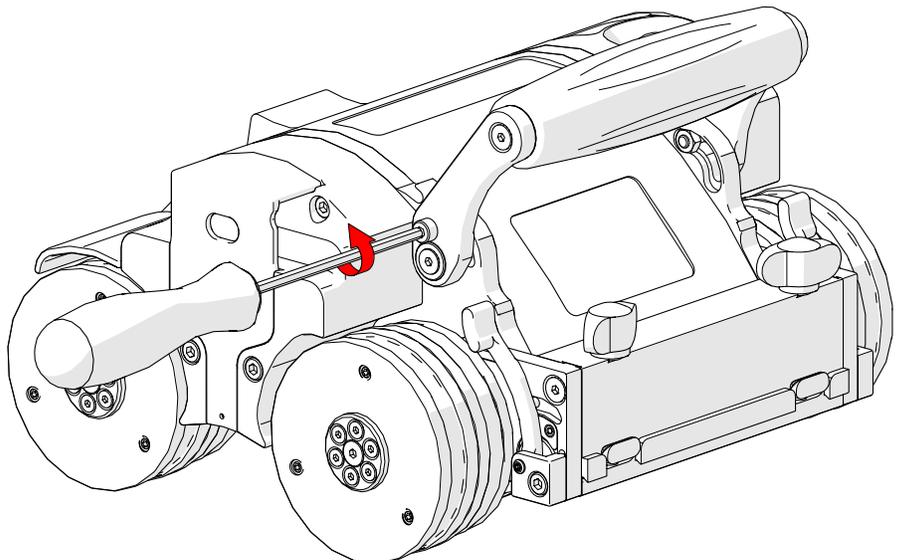


Fig. 93 - Unscrew handle lock screw

1. To lower the handle, use the supplied 3 mm driver to loosen the handle lock screws on either side of the handle (Fig. 93).

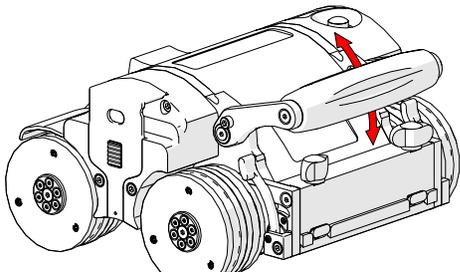


Fig. 94 - Pivot handle as desired

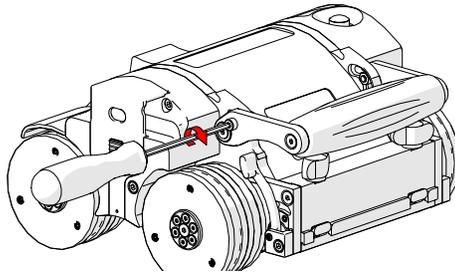


Fig. 95 - Tighten lock screws

2. Pivot the handle as required (Fig. 94).
3. Tighten the handle lock screws when complete (Fig. 95).

5.6.4. Emergency Off Button

The red button located on the top left of the crawler provides an emergency off button to the entire system. When pressed, all power to the **SKOOT** system will disengage.

To restore system power, it is necessary to press the green power button located on the power controller (see "Power Controller" on page 26).




Fig. 96 - Emergency off

NOTE: Terminating system power may cause the crawler to freewheel down when operating in a vertical orientation.

5.6.5. Cable Retainer

Located at the on the side of the crawler, the cable retainer offers a means of cable management for cables, hoses and tubes. Gently apply pressure to the grooves of the cable retainer and lift (Fig. 97). Route cables, hoses or tubes through the retainer and then press the cable retainer down (Fig. 98).

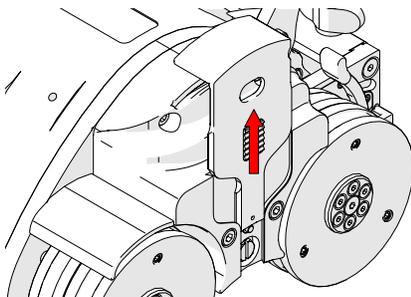


Fig. 97 - Lift retainer by hand

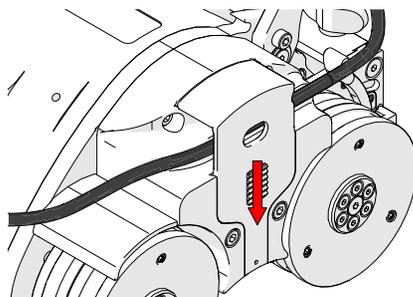


Fig. 98 - Place cables and hoses then close retainer

5.6.6. Manipulation Handle

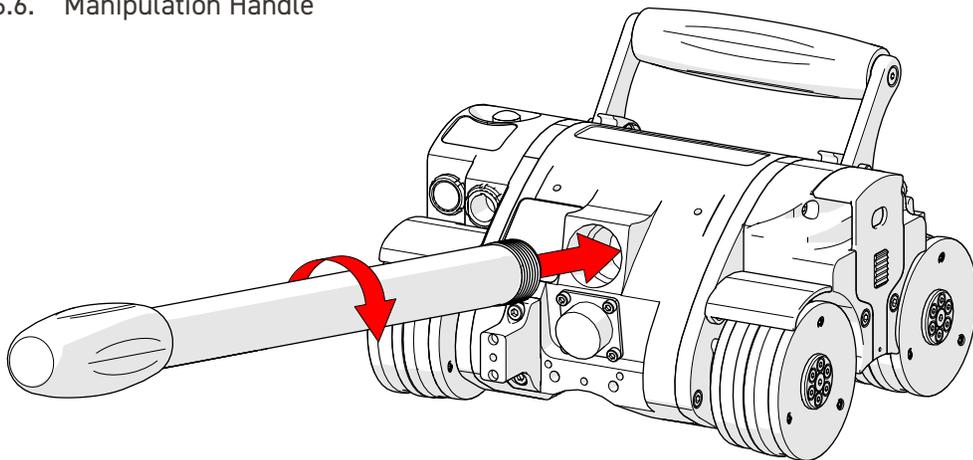


Fig. 99 - Manipulation handle

The manipulation handle (Fig. 99) provides a means of orienting the scanner direction. The handle can be used to set initial scanner direction as well as occasional orientation correction. The manipulation handle is not intended as a tool for constant adjustment during a scan operation.

The handle may be removed when additional scanner clearance is required.

NOTE: Do not use the manipulation handle to remove or install a crawler from a scan surface without the installation/removal mat in place.

5.7. Backpack

The **SKOOT** backpack provides a mounting point for scanning peripherals. The flexible strap securely holds any preamp, splitters or scan accessories to the **SKOOT** crawler.

5.7.1. Mounting a Backpack

To mount the backpack, follow these steps.

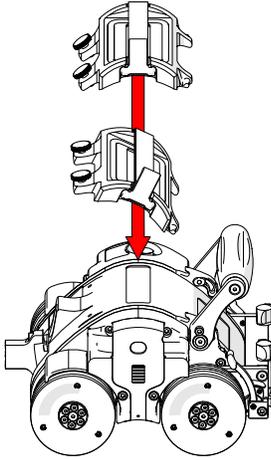


Fig. 100 - Angle backpack

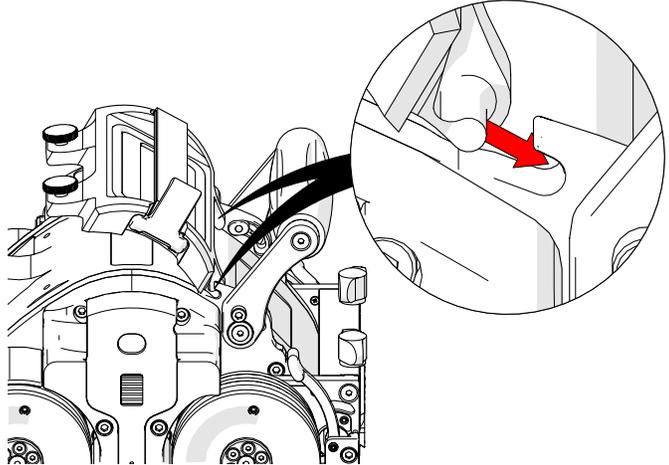


Fig. 101 - Fit backpack into notches

1. Angle the backpack (Fig. 100) towards the notches found on the **SKOOT** (located near the base of the handle).
2. Place the front of the backpack into the notches found near the base of the handle (Fig. 101).
3. Lower the backpack to the **SKOOT** and tighten the thumb screws to secure the backpack (Fig. 102).

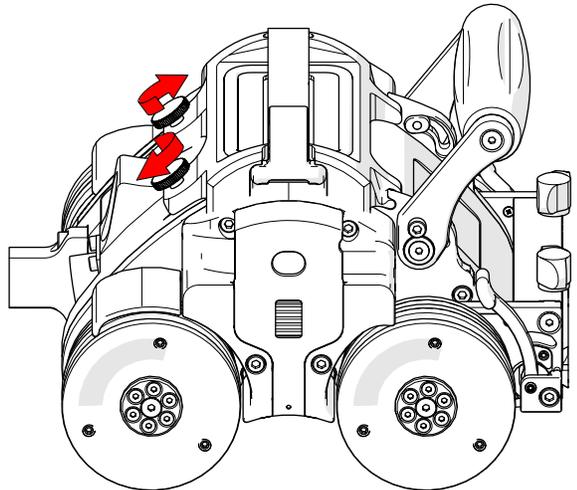


Fig. 102 - Tighten thumb screws

5.7.2. Using the backpack

The flexible strap of the backpack stretches to hold various scanning accessories to crawler.

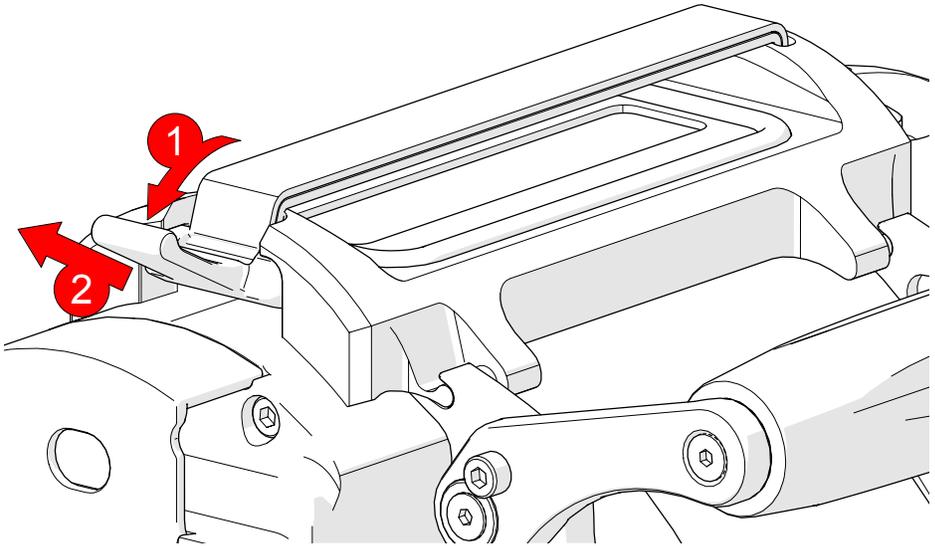


Fig. 103 - Press lever down and pull to release

1. Press the strap's lever down (*Fig. 103-1*) and then pull (*Fig. 103-2*) to release the flexible strap.

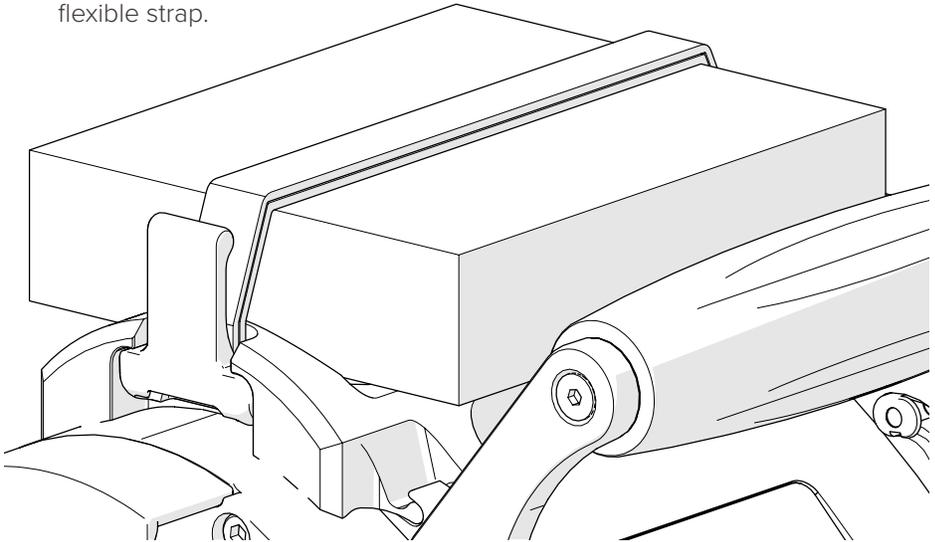


Fig. 104 - Press lever into backpack to lock in place

2. Place the scanning accessory on the backpack. Pull the strap lever across the accessory and fit the lever into place on the backpack (*Fig. 104*).

5.8. Probe Holders

5.8.1. Heavy Duty Vertical Probe Holder

- A Latch
- B Probe Holder Arm Adjustment Knob
- C Yoke
- D Probe Holder Arms
- E Pivot Buttons
- F Arm Clamp Screw
- G Probe Holder Adjustment Knob
- H Vertical Adjustment Knob

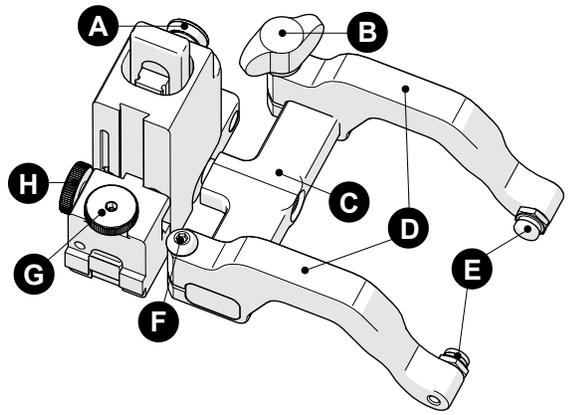


Fig. 105 - Heavy duty vertical probe holder

5.8.1.1 Probe Holder Setup

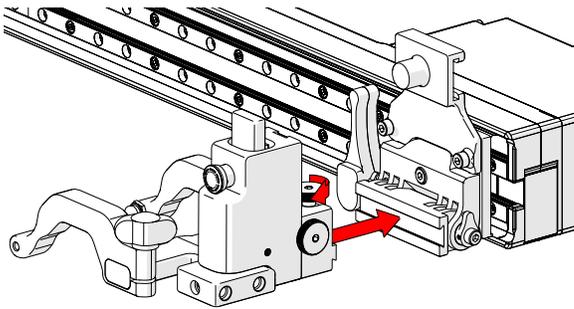


Fig. 106 - Mount probe holder to carrier

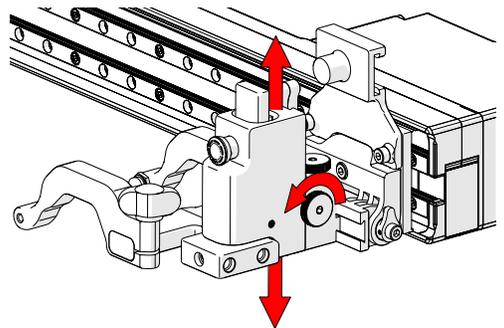


Fig. 107 - Vertical adjustment

1. Loosen the probe holder adjustment knob (*Fig. 106*) and mount the heavy duty vertical probe holder's dovetail jaw to the carrier.
2. The vertical adjustment knob (*Fig. 107*) allows the heavy duty vertical probe holder's height adjustment. This adjustment also controls the probe holders spring tension.

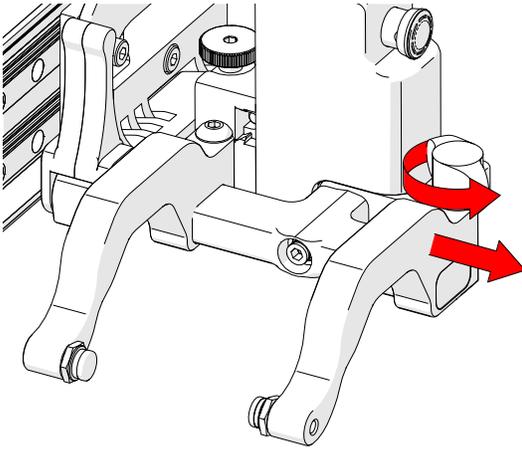


Fig. 108 - Remove outer arm

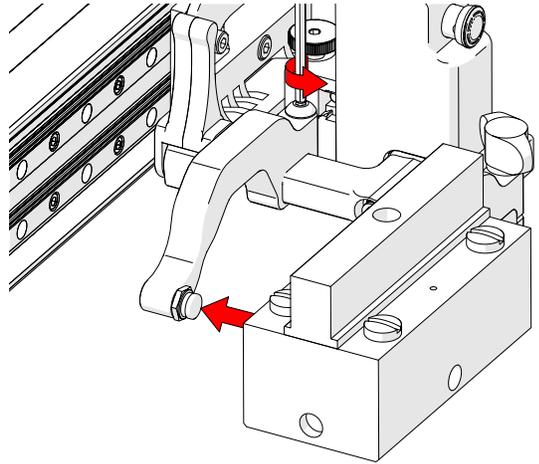


Fig. 109 - Adjust inner arm

3. Loosen the probe holder adjustment knob and remove the outer probe holder arm (Fig. 108).
4. Loosen the arm clamp screw (Fig. 109).
5. Place the wedge on the pivot button of the inner probe holder arm (Fig. 108).

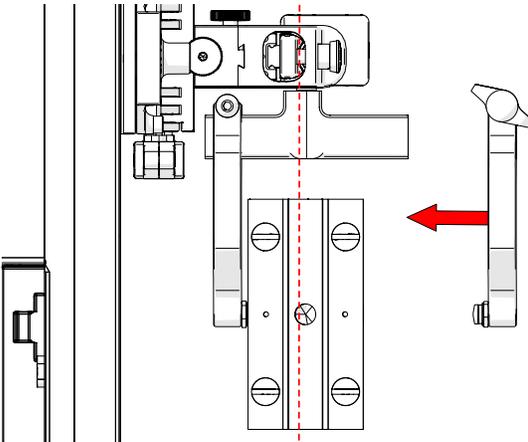


Fig. 110 - Align probe with yoke

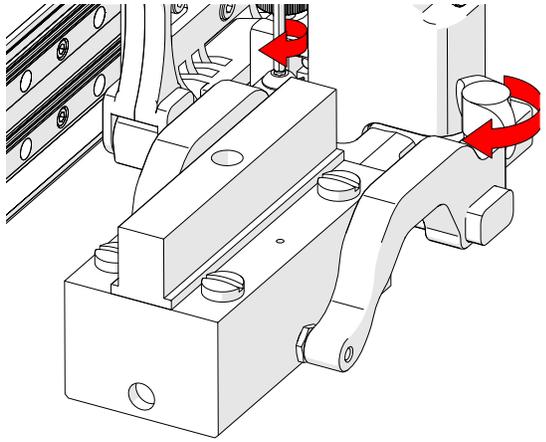


Fig. 111 - Tighten knobs and screws

6. Align the middle of the wedge with the centre of the yoke (Fig. 110).
7. Tighten both the probe holder adjustment knob and the arm clamp screw (Fig. 111) while ensuring the wedge remains centred with the yoke.

5.8.1.2 Probe Holder Vertical Adjustment

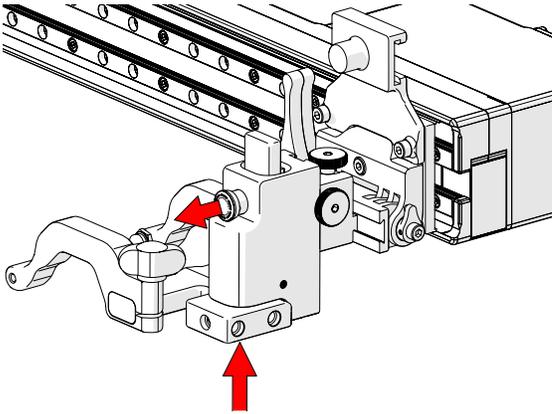


Fig. 112 - Press up and pull latch

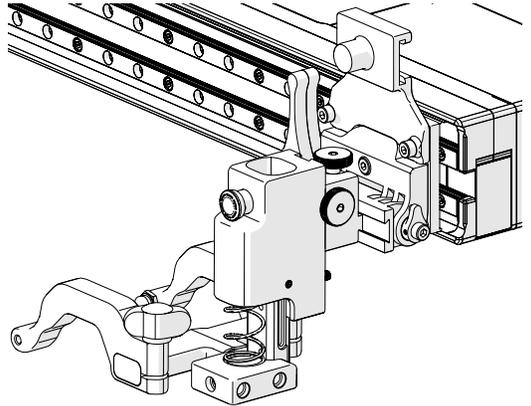


Fig. 113 - Lowered toward scan surface

1. Gently lift the heavy duty vertical probe holder and simultaneously pull the latch (*Fig. 112*). This action will unlock the probe holder. Slowly lower the probe holder towards the scan surface (*Fig. 113*).

5.8.1.3 Probe Holder Left/Right Conversion

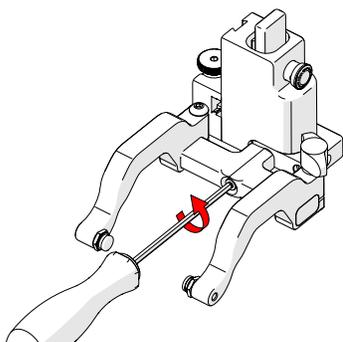


Fig. 114 - Remove yoke

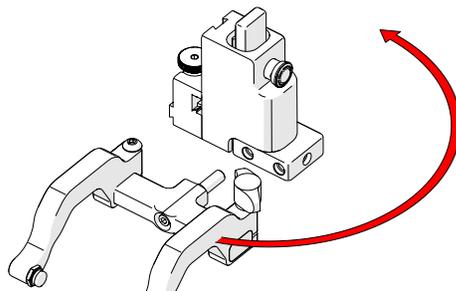


Fig. 115 - Orient to opposite side

1. Using the supplied 3 mm driver, unscrew the yoke (Fig. 114).
2. Position the yoke and arms to the opposite side of the probe holder (Fig. 115).

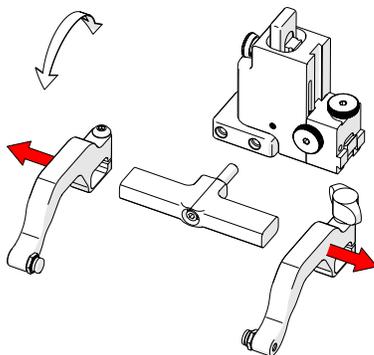


Fig. 116 - Remove probe holder arms

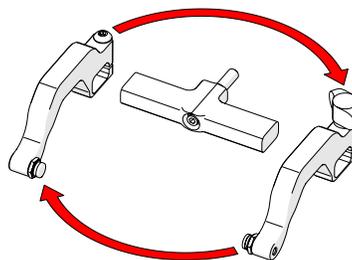


Fig. 117 - Reverse position around yoke

3. Loosen the arm clamp screw and the probe holder arm adjustment knob allowing removal of the probe holder arms (Fig. 116).
4. Position the removed arms to the opposite sides of the yoke (Fig. 117).

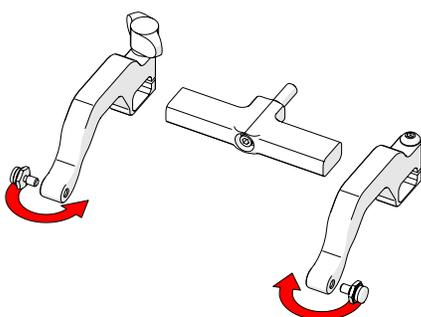


Fig. 118 - Position pivot buttons

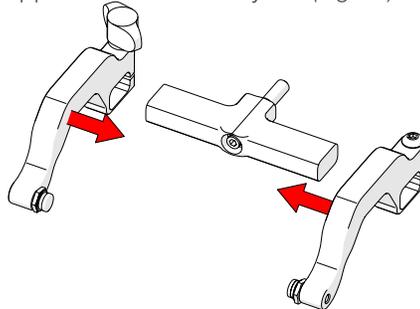


Fig. 119 - Place arms back onto yoke

5. Position the pivot buttons to the inside of the probe holder arms (Fig. 118).
6. Place the probe holder arms on the yoke and tighten the arm clamp screw and probe holder adjustment knob (Fig. 119).
7. Screw the yoke to the probe holder (Fig. 120).

TIP: When using a standard yoke length, position the yoke in the threaded hole closest to the frame bar. When using a long yoke length, position the yoke in the threaded hole furthest from the frame bar.

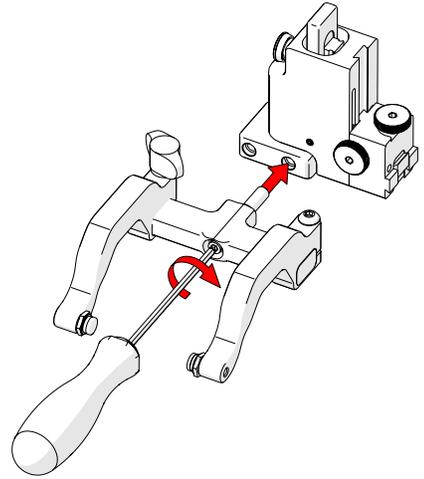


Fig. 120 - Screw into threaded hole

5.8.1.4 Probe Holder 90° Adjustment

1. Remove the yoke using the supplied 3 mm hex driver (Fig. 114).
2. Orient the yoke to the front of the probe holder and screw the yoke into the threaded hole provided (Fig. 121).

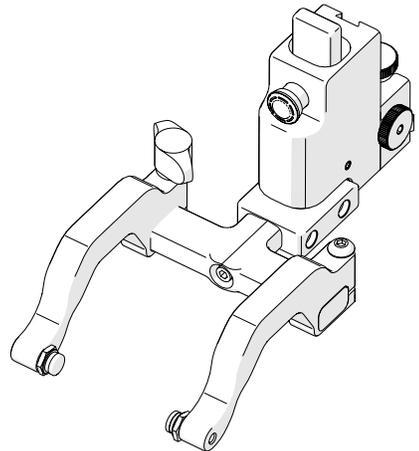


Fig. 121 - 90° probe holder positioning

5.8.2. Vertical Probe Holder

- A Latch
- B Probe Holder Adjustment Knob
- C Vertical Adjustment Knob
- D Pivot Buttons
- E Probe Holder Arms
- F Yoke
- G Probe Holder Arm Adjustment Knob
- H Transverse Adjustment Screw
- I Frame Bar

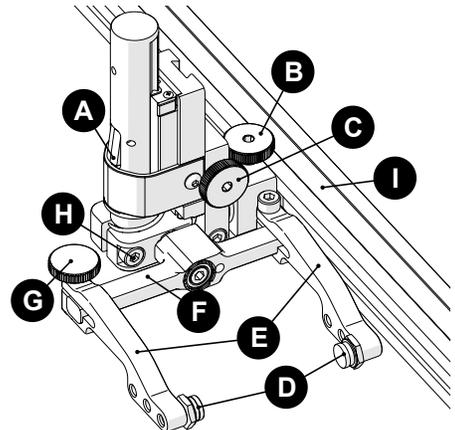


Fig. 122 - Vertical probe holder

5.8.2.1 Probe Holder Setup

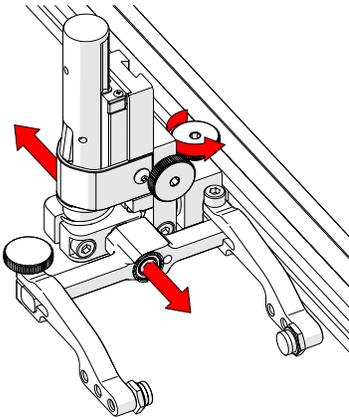


Fig. 123 - Adjust on frame bar

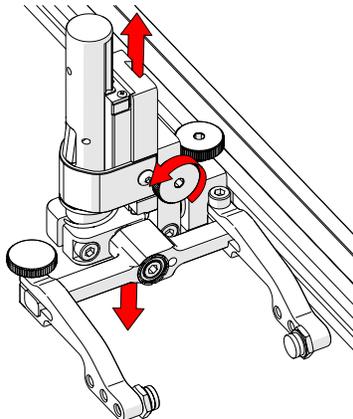


Fig. 124 - Vertical adjustment

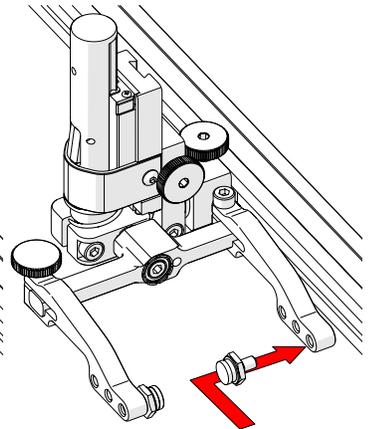


Fig. 125 - Place buttons

1. The probe holder adjustment knob allows the probe holder to be attached to a frame bar, as well as horizontal positioning on a frame bar (Fig. 123).
2. The vertical adjustment knob allows the vertical probe holder height adjustment (Fig. 124).
3. Position the pivot buttons where necessary. When a narrow scanning footprint is required, use the pivot button holes closest to the yoke (Fig. 125).

TIP: Probe pivoting may be impeded when closer to the yoke.

To mount a UT wedge in the probe holder, follow these steps:

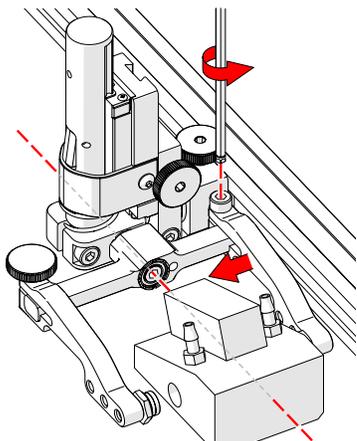


Fig. 126 - Adjust inner arm

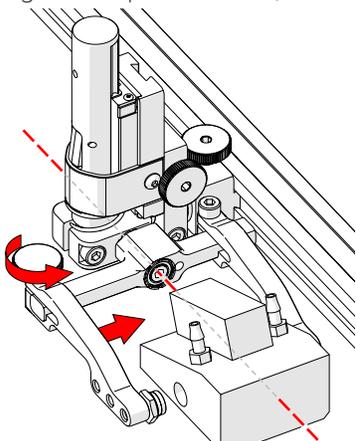


Fig. 127 - Adjust outer arm

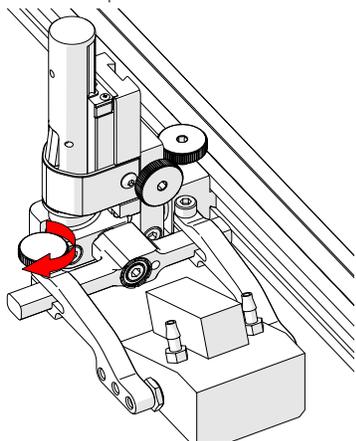


Fig. 128 - Tighten arm knob

2. Position the wedge on the inner probe holder arm (Fig. 126).

TIP: The probe holder yoke can accommodate many different probe and wedge sizes of varying widths. It is best to centre the wedge with the yoke's pivot axis. This can reduce wedge 'rocking' when scanning. Position the inner probe holder arm accordingly (Fig. 126) using the supplied 3 mm hex driver (Fig. 42).

3. Loosen the probe holder arm adjustment knob (Fig. 127) and slide the probe holder arm along the yoke pinching the wedge in place.
4. Tighten the probe holder arm adjustment knob (Fig. 128).

5.8.3. Probe Holder Vertical Adjustment

To adjust the probe holder vertically, follow these steps:

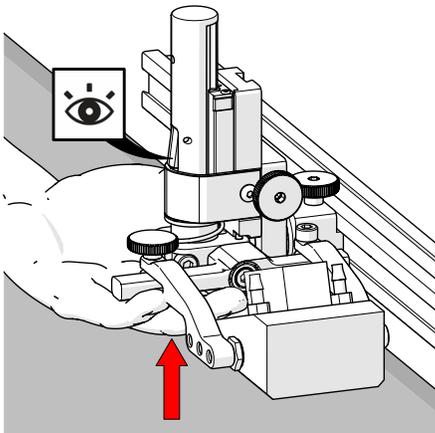


Fig. 129 - Latch probe holder

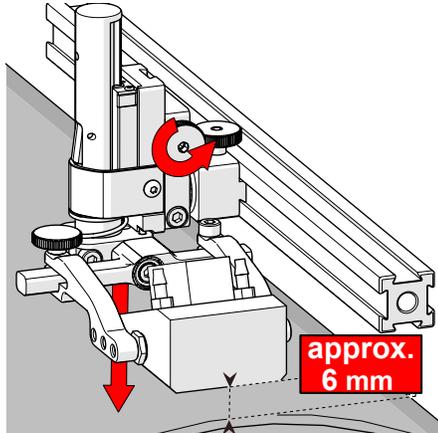


Fig. 130 - Lower toward scan surface

1. Ensure the probe holder is in the latched, upper position. Lift the probe holder until the latch is fully exposed and snaps out to lock (Fig. 129).
2. Loosen the vertical adjustment knob and slide the probe holder down until the wedge is approximately 6 mm ($\frac{1}{4}$ in) above inspection surface.
3. Tighten the vertical adjustment knob (Fig. 130).

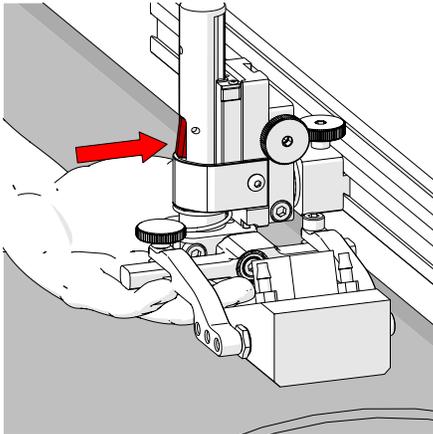


Fig. 131 - Press latch button

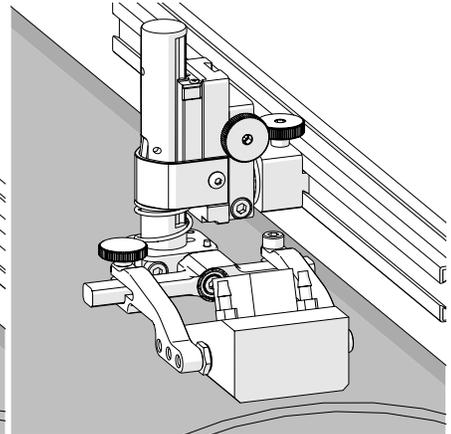


Fig. 132 - Lower toward scan surface

4. Lift the yoke slightly and press the latch button (Fig. 131), then slowly lower towards scanning surface to apply spring pressure to the wedge (Fig. 132).

TIP: If less spring force is desired, refer to step 2 and place the wedge approximately 20 mm ($\frac{3}{4}$ in) above inspection surface.

5.8.4. Probe Holder Transverse Adjustment

To adjust the probe holder's transverse angle, follow these steps:

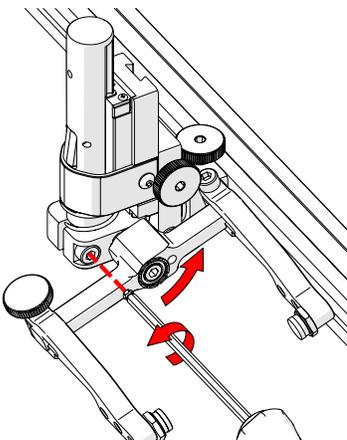


Fig. 133 - Loosen 3 mm screw

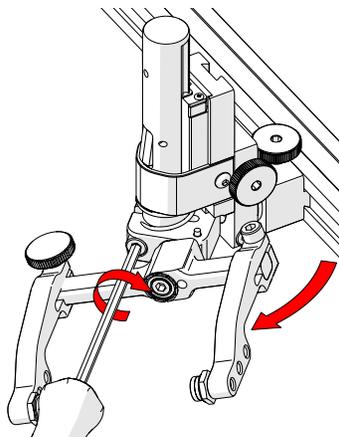


Fig. 134 - Rotate and tighten

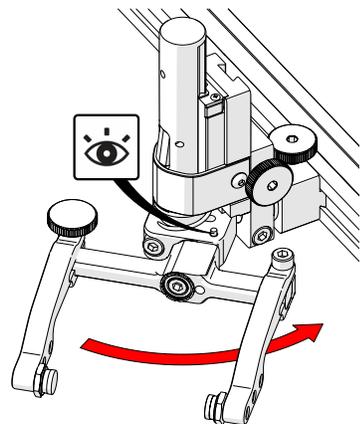


Fig. 135 - Stop post locates 90°

1. Ensure the probe holder is in latched, upper position (*Fig. 129*).
2. Using the supplied 3 mm hex driver loosen the transverse adjustment screw (*Fig. 133*) and rotate the yoke about the vertical shaft achieving the desired angle.
3. Tighten the transverse adjustment screw (*Fig. 134*).

To return the transverse adjustment to neutral (90°). The probe holder must be in the latched, upper position (*Fig. 129*). Rotate the yoke until the stop post contacts the base of the probe holder (*Fig. 135*). Then tighten the transverse adjustment screw.

5.8.5. Probe Holder Longitudinal Adjustment

To adjust the probe holder's vertical angle for longitudinal scanning, follow these steps:

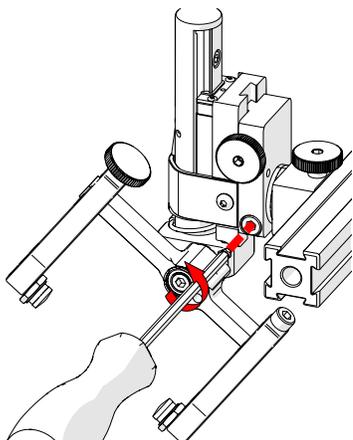


Fig. 136 - Loosen 3 mm screw

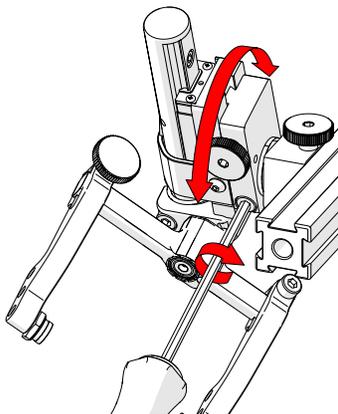


Fig. 137 - Rotate to position

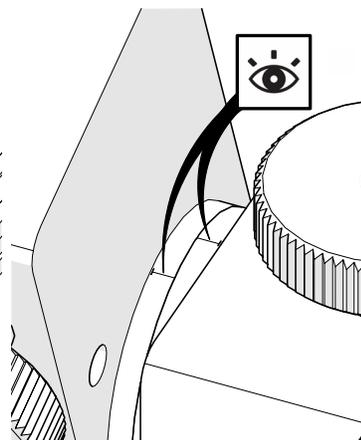


Fig. 138 - Line up markers

1. Ensure the probe holder is in latched, upper position (*Fig. 129*).
2. Using the supplied 3 mm hex driver (*Fig. 42*), loosen the longitudinal adjustment screw (*Fig. 136*).
3. Rotate the main body of the probe holder until it is at the desired angle (*Fig. 137*).
4. Tighten the longitudinal adjustment screw (*Fig. 137*).

To return the longitudinal adjustment to neutral (90°). Line up the longitudinal adjustment indicator markers (*Fig. 138*).

5.8.6. Probe Holder Left/Right Conversion

To reverse the probe holder, follow these steps:

NOTE: To perform this operation the 1.5 mm hex wrench (Fig. 45) is required.

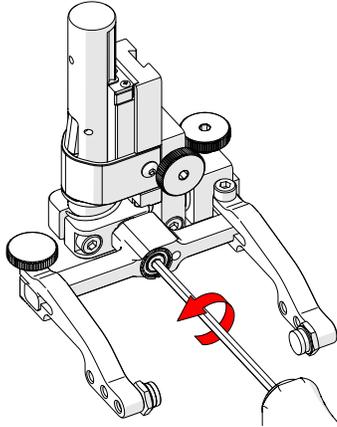


Fig. 139 - Unscrew yoke pivot screw

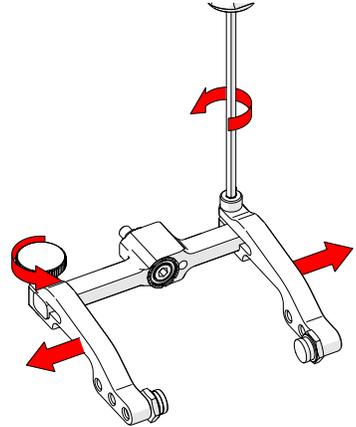


Fig. 140 - Remove probe holder arms

1. Ensure the probe holder is in latched, upper position (Fig. 129).
2. Using the supplied 3 mm hex driver (Fig. 42), unscrew the yoke pivot screw and remove yoke (Fig. 139).
3. Loosen the probe holder arm adjustment knob and the arm clamp screw. Slide the probe holder arms off the yoke (Fig. 140).

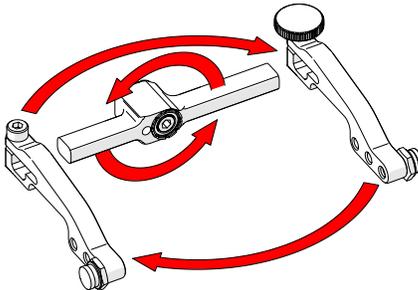


Fig. 141 - Flip yoke and reverse arms

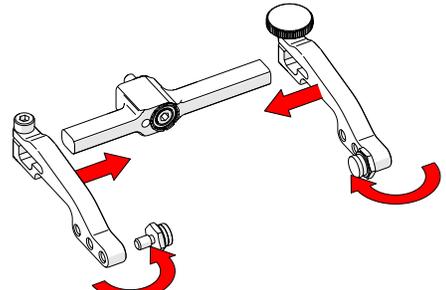


Fig. 142 - Attach arms & move buttons

4. Flip the yoke 180° and reverse the probe holder arms (Fig. 141).
5. Place the pivot buttons on the inside of the probe holder arms (Fig. 142) using a 3/8 in wrench (Fig. 43).

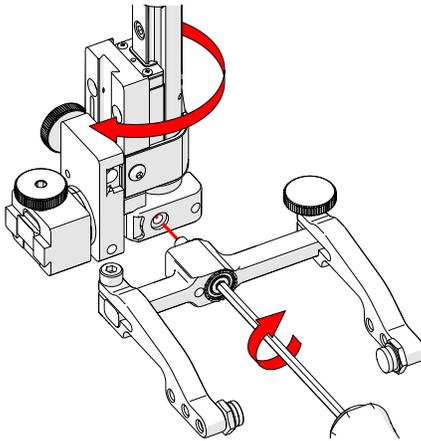


Fig. 143 - Screw yoke to opposite side

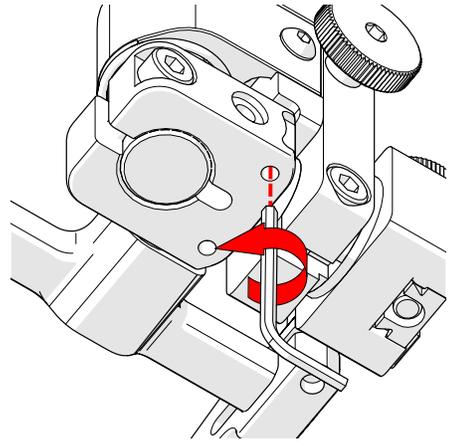


Fig. 144 - Lower 90° stop post

6. Mount the yoke to the opposite side of the base using the supplied 3 mm hex driver (Fig. 143).

TIP: Keep the yoke level with the base as to ensure no conflicts with the plunger/set screw attached to the yoke.

7. Locate the recessed M3 screw on the bottom of the probe holder. Unscrew the stop post using a 1.5 mm hex wrench (Fig. 45) until it has cleared all obstructions. Do not remove stop post (Fig. 144).

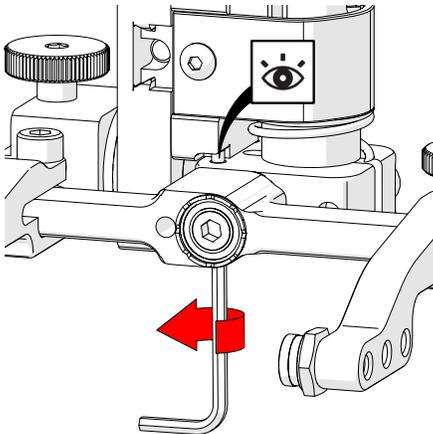


Fig. 145 - Raise opposite 90° stop post


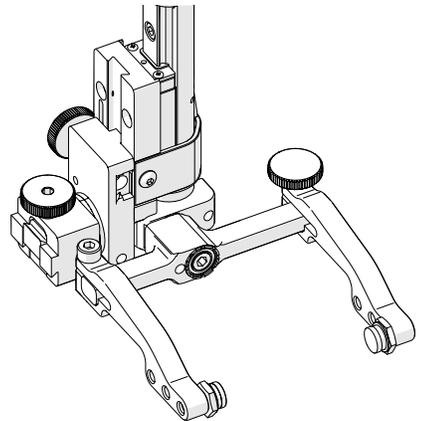


Fig. 146 - Reversed probe holder

8. Raise the stop post on the opposite side until the side of the post clearly contacts the 90° stop point on the probe holder's base (Fig. 145).

5.9. Slip Joint Probe Holder

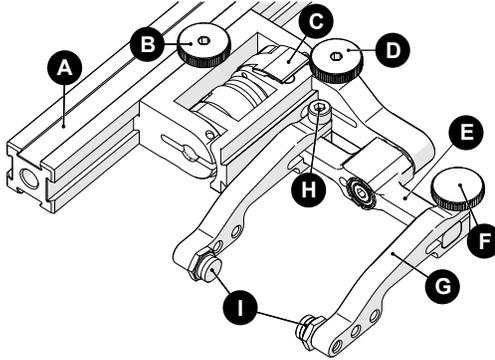

A	Frame Bar
B	Probe Holder Adjustment Knob
C	Latch
D	Swing Arm Knob
E	Yoke
F	Probe Holder Arm Adjustment Knob
G	Probe Holder Arm
H	Arm Clamp Screw
I	Pivot Buttons

Fig. 147 - Slip Joint Probe Holder

5.9.1. Probe Holder Setup

To mount a UT wedge in the probe holder, follow these steps:

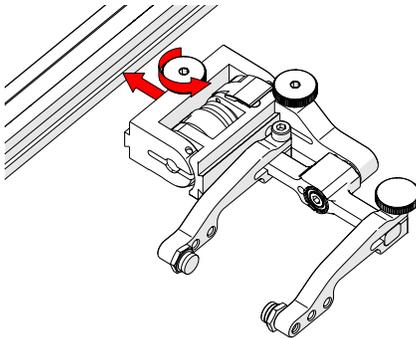


Fig. 148 - Attach to frame bar

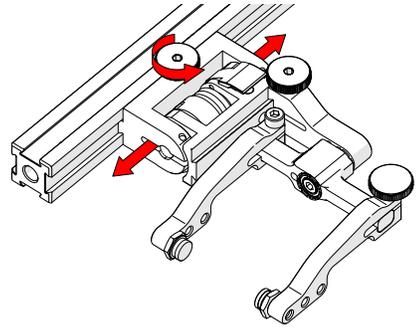


Fig. 149 - Adjust on frame bar

1. Rotate the probe holder adjustment knob and attach probe holder to a frame bar (Fig. 148).
2. Use the probe holder adjustment knob to position the probe holder along the frame bar (Fig. 149).

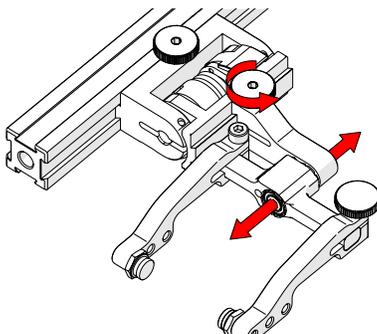


Fig. 150 - Adjust swing arm

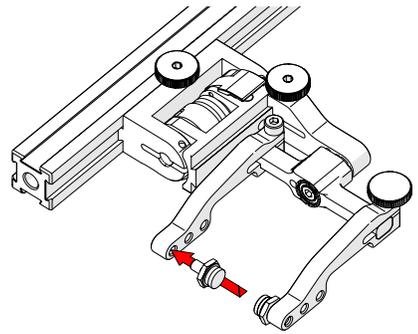


Fig. 151 - Place pivot buttons

3. Use swing arm knob to position the swing arm (Fig. 150).

TIP: The swing arm is typically used to adjust TOFD center to center distance relative to the phased array probes on a four probe configuration.

4. Using the supplied 3/8 in wrench, place the pivot buttons (Fig. 151) farthest from the yoke for maximum wedge clearance.

TIP: If narrow scanning footprint is required, use pivot button holes closest to the yoke. Wedge pivoting may be impeded when closer to the yoke.

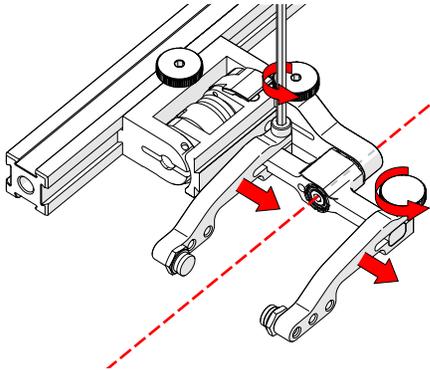


Fig. 152 - Adjust probe holder arms

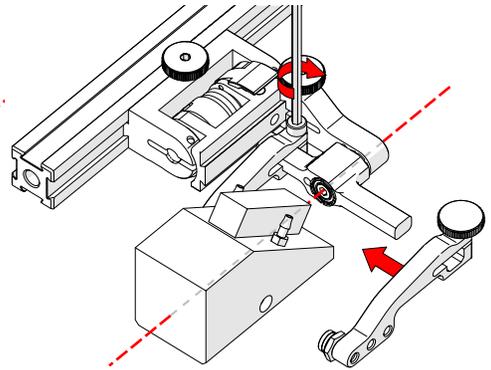


Fig. 153 - Place wedge

5. Loosen the probe holder arm adjustment knob (Fig. 152) and remove outer probe holder arm from yoke.
6. Adjust inner probe holder arm as required to best centre the probe on the yoke's pivot axis (Fig. 152).

TIP: The probe holder yoke can accommodate many different probe and wedge sizes of varying widths. It is best to centre the wedge with the yoke's pivot axis to reduce wedge tipping when scanning. Position the inner probe holder arm accordingly with the centre of the yoke (Fig. 152).

7. Position the wedge on the inner probe holder arm (Fig. 153).
8. Slide outer probe holder arm along the yoke pinching the wedge in place.
9. Tighten probe holder arm adjustment knob (Fig. 154).

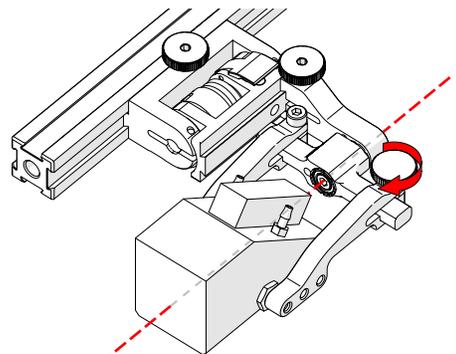


Fig. 154 - Pinch wedge with arm

5.9.2. Probe Holder Adjustment

To adjust the probe holder, follow these steps:

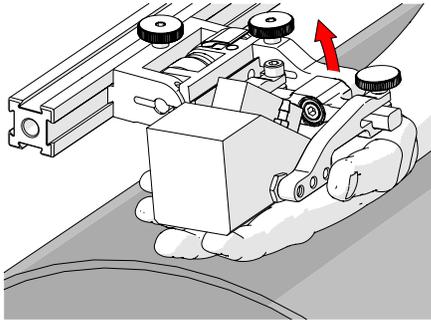


Fig. 155 - Lift to latched position

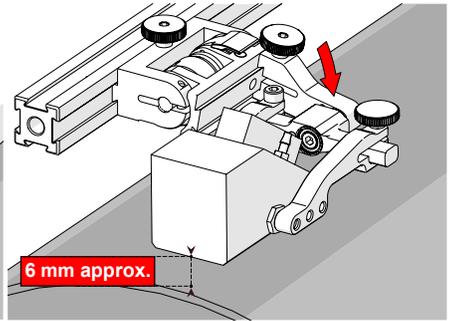


Fig. 156 - Lower to scanning surface

1. Ensure probe holder is in latched, upper position (Fig. 155). If the probe holder is already latched, it will only move within the slip joint adjustment range and have no spring tension.
2. Push the probe holder yoke down toward inspection surface until the wedge is approximately 6 mm ($\frac{1}{4}$ in) above the inspection surface (Fig. 156).

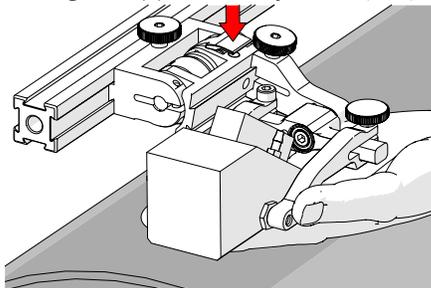


Fig. 157 - Lift and press latch button

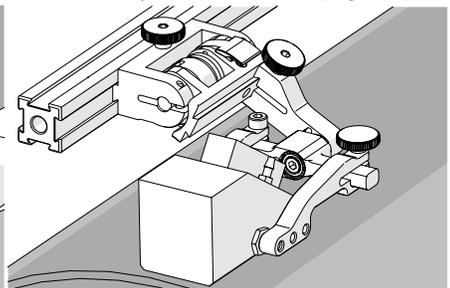


Fig. 158 - Spring loaded scan position

3. Lift probe slightly and press latch button (Fig. 157) to apply spring pressure to the wedge.
4. Gently lower probe holder and wedge to the scanning surface (Fig. 158).

5.9.3. Probe Holder Force Adjustment

It is possible to adjust the tension of the probe holder spring.

NOTE: To perform this operation the 2 mm hex wrench (Fig. 46) and 3 mm hex wrench (Fig. 42) is required.

Light	1 kg	2 lb
Medium	2 kg	4 lb
Heavy	3 kg	6 lb

When configured correctly, these settings exert the indicated spring force on the Probe.

To adjust the probe holder's force, follow these steps:

NOTE: Do not perform this operation on scanning surface.

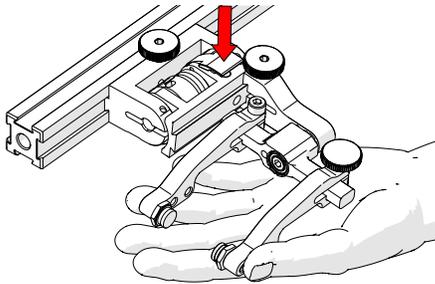


Fig. 159 - Lift slightly and press Latch

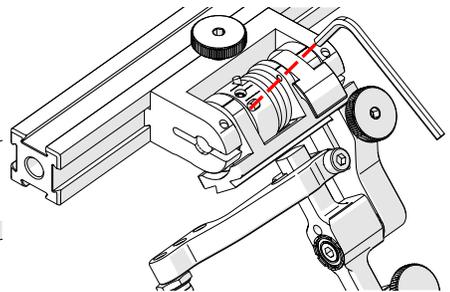


Fig. 160 - Unlatched position

1. Ensure the probe holder is in the upright latched position (Fig. 155).
2. Lift probe holder slightly and press the latch button (Fig. 159) to release the probe holder the full 45° degrees.
3. Insert the short arm of a 3 mm hex wrench into the 3 mm slot (Fig. 160).

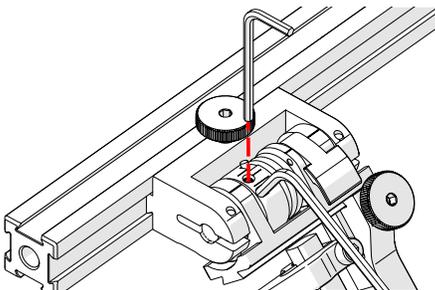


Fig. 161 - Insert hex tools

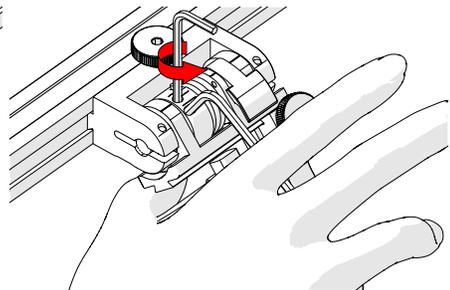


Fig. 162 - Press 3 mm hex wrench down

4. Place the 2 mm hex wrench into the force adjustment screw (Fig. 161).
5. Lightly press the long arm of the 3 mm hex wrench down. Using the 2 mm hex wrench, loosen the force adjustment screw but do not remove it (Fig. 162).
6. Gently apply pressure on the long leg of the 3 mm hex wrench until the force adjustment marker lines up with the desired spring tension. While keeping the markers in line, tighten the force adjustment screw.

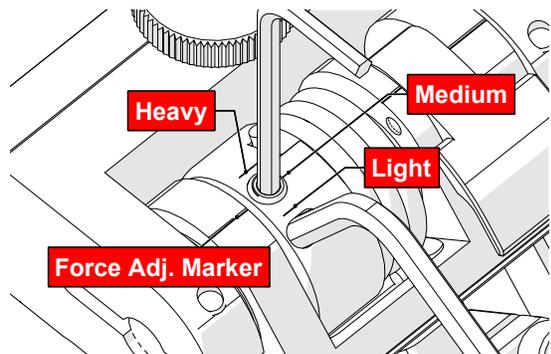


Fig. 163 - Choose desired tension

5.9.4. Slip Joint Probe Holder Left/Right Conversion

To reverse the probe holder, follow these steps:

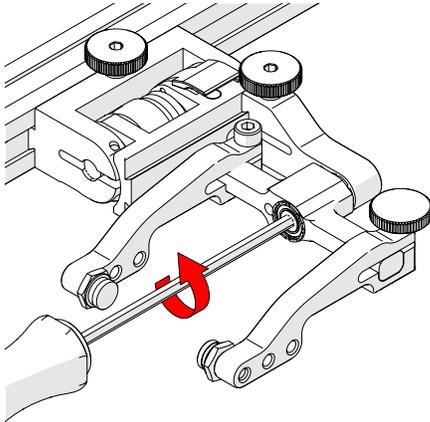


Fig. 164 - Unscrew yoke pivot screw

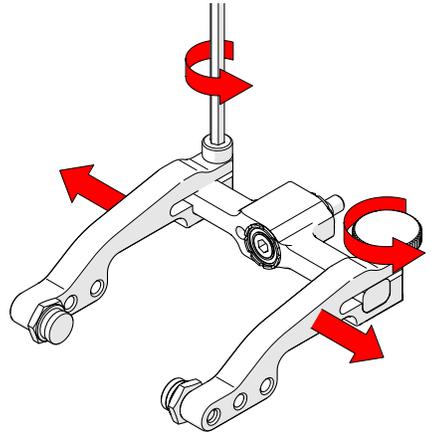


Fig. 165 - Remove arms

1. Unscrew the yoke from the swing arm (Fig. 164).
2. Loosen the probe holder arm adjustment knob and arm clamp screw. Slide the arms from the yoke (Fig. 165).

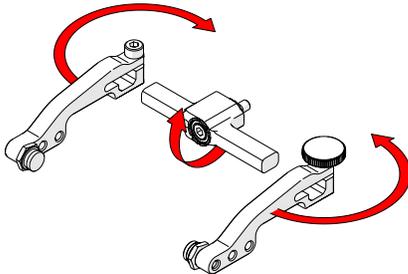


Fig. 166 - Flip yoke and reverse arms

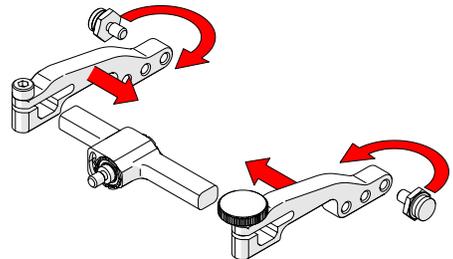


Fig. 167 - Attach arms and move buttons

3. Flip the yoke 180° and reverse the probe holder arms (Fig. 166).
4. Place the pivot buttons on the inside of the probe holder arms (Fig. 167) using a 3/8 in wrench (Fig. 43). Slide the arms onto the yoke and tighten the probe holder arm adjustment knob and the arm clamp screw.

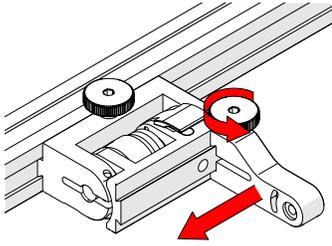


Fig. 168 - Position swing arm

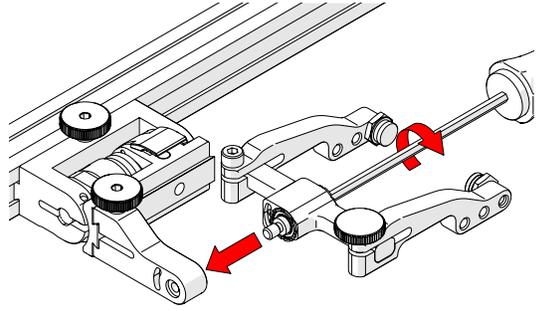


Fig. 169 - Install yoke to swing arm

5. Loosen the swing arm knob and slide the swing arm to the opposite end of the probe holder bracket (*Fig. 168*) or preferred position. Tighten swing arm knob.
6. Using the 3 mm hex driver, screw the yoke pivot screw into the opposite side of the probe holder swing arm (*Fig. 169*). Ensure the yoke is level to avoid issues with the plunger/set screw.

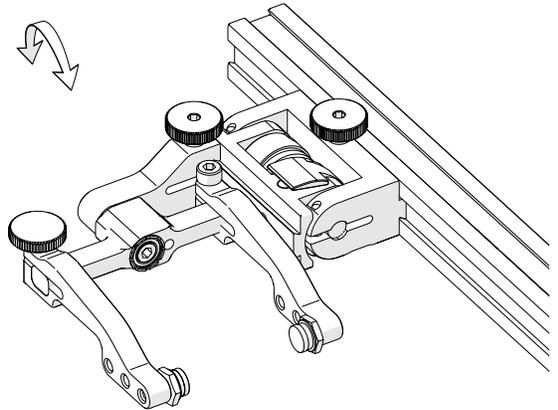


Fig. 170 - Reversed probe holder

5.10. Probe Holder Frames

5.10.1. Low Profile Probe Holder Frame - Flat or Circumferential Only



WARNING! FALLING OBJECT HAZARD.

It is imperative that the steps below be followed to properly set the height of the probe holder frame. If the height of the probe holder frame is set too low, the crawler may fall and **SEVERE INJURY** or **DEATH** could result.

The low profile frame adds weld scanning capability to the **SKOOT** motorized scanner. This frame can utilize (4) slip joint probe holders (2 Phased Array and 2 TOFD, typically). The low profile design of this frame allows for scanning on diameters where radial clearance is limited.

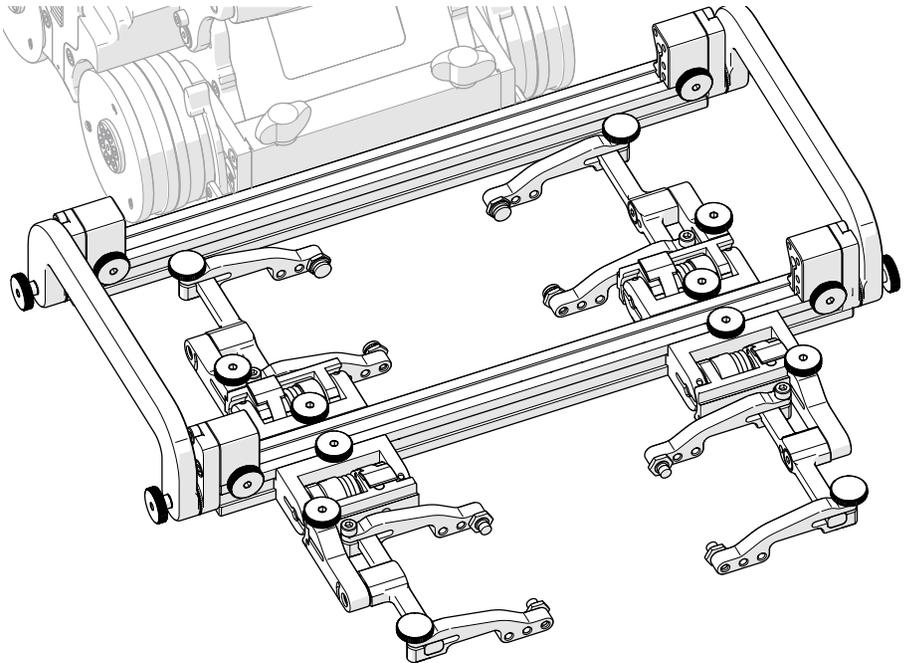


Fig. 171 - Low profile probe holder frame

1. Attach the wedges to the probe holders that are to be used (see *Probe Holder Setup* on page 60 for additional details).

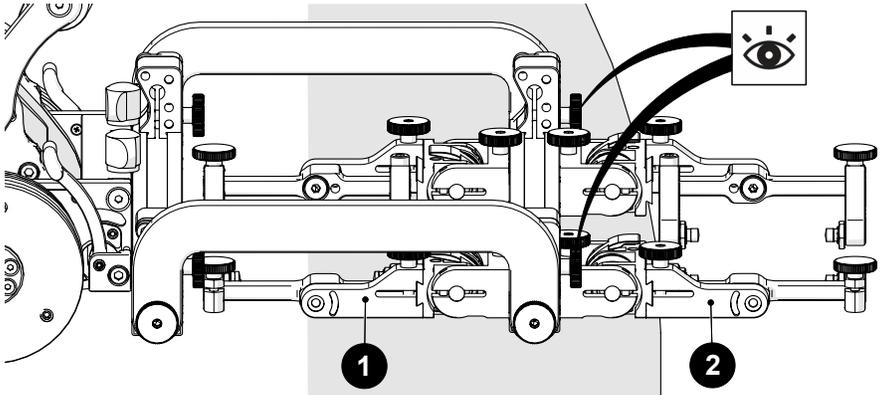


Fig. 172 - Position primary and secondary probe holders

2. Affix the probe holders (with attached wedges) to the low profile probe holder frame. On the frame bar, place the secondary probe holders at the front (Fig. 172-2) and the primary probe holders at the rear (Fig. 172-1).

TIP: Due to their larger size, scan results are generally improved when pulling or dragging phased array wedges.

3. Mount the low profile probe holder frame to the crawler (see *Cable Retainer* on page 51 for additional details). When mounting the low profile frame, ensure the attachment knobs (Fig. 172) are at the front (non crawler side).

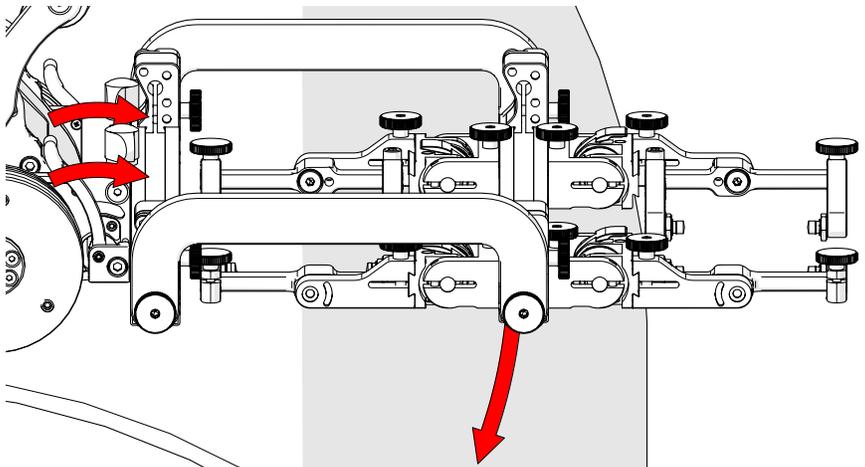


Fig. 173 - Align swivel mount with scan surface

4. Release the two swivel mount levers (Fig. 173) to position the swivel mount parallel to the scan surface (Fig. 174). When alignment with scan surface is achieved, lock the crawler swivel mount levers.

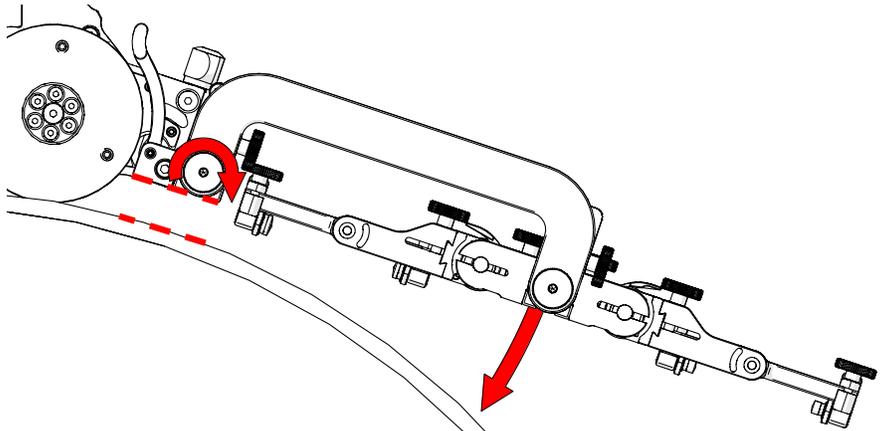


Fig. 174 - Set rear rotational adjustment knob

5. Loosen the rear rotational adjustment knob to lower the front frame bar of the low profile frame towards the inspection surface (*Fig. 174*).


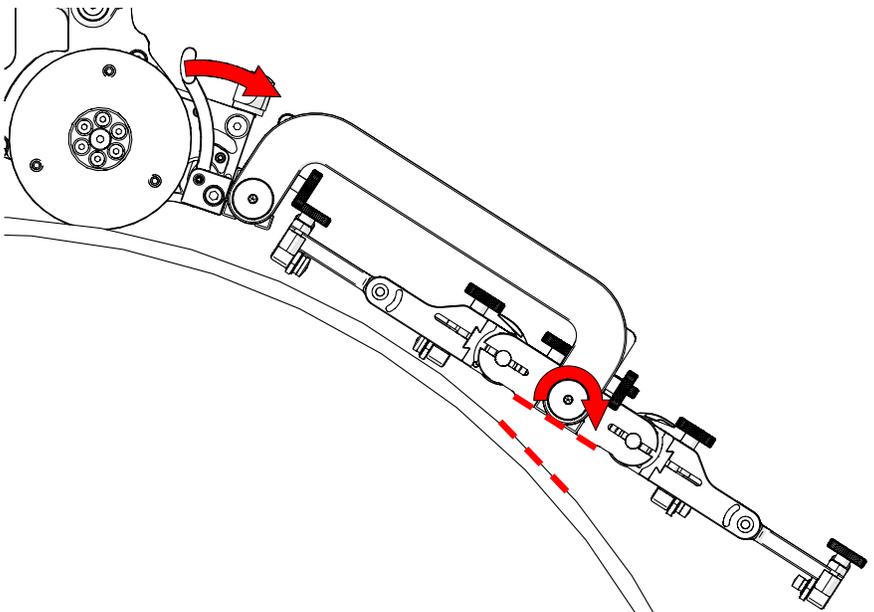


Fig. 175 - Align probe holder tangent with scan surface

6. Loosen the front rotational adjustment knob (*Fig. 175*) to align the frame bar parallel with the scan surface (*Fig. 176*).

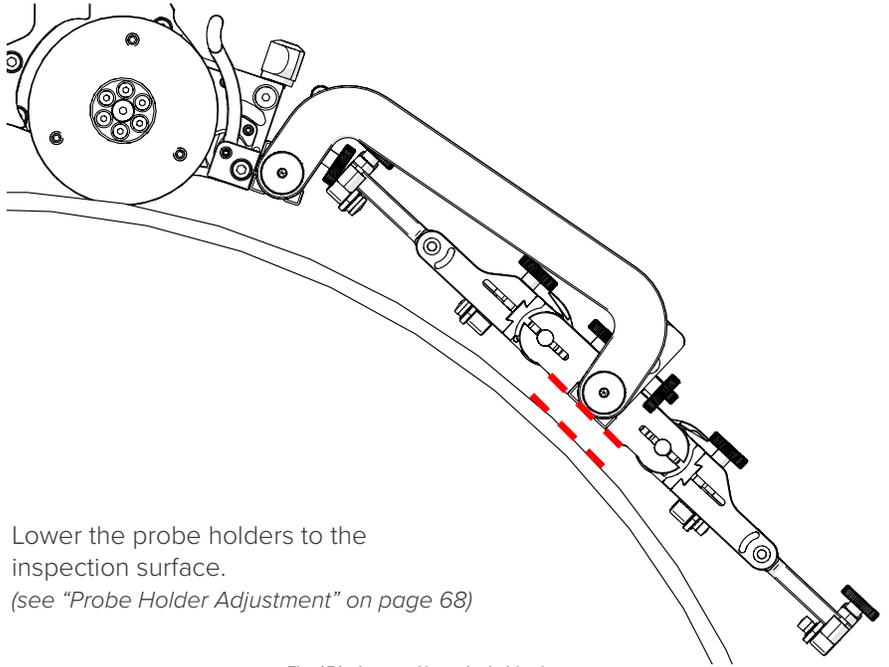

7. Lower the probe holders to the inspection surface.
(see "Probe Holder Adjustment" on page 68)

Fig. 176 - Low profile probe holder frame

5.10.2. Vertical Probe Holder Frame - Flat or Circumferential Only



WARNING! FALLING OBJECT HAZARD.

It is imperative that the steps below be followed to properly set the height of the probe holder frame. If the height of the probe holder frame is set too low, the crawler may fall and **SEVERE INJURY** or **DEATH** could result.

The vertical probe holder frame adds weld scanning capability to the **SKOOT** motorized scanner. This frame uses (4) vertical probe holders. Additional frame components allow up to six probes to be used (*contact Jireh Industries Ltd. on page 3*).

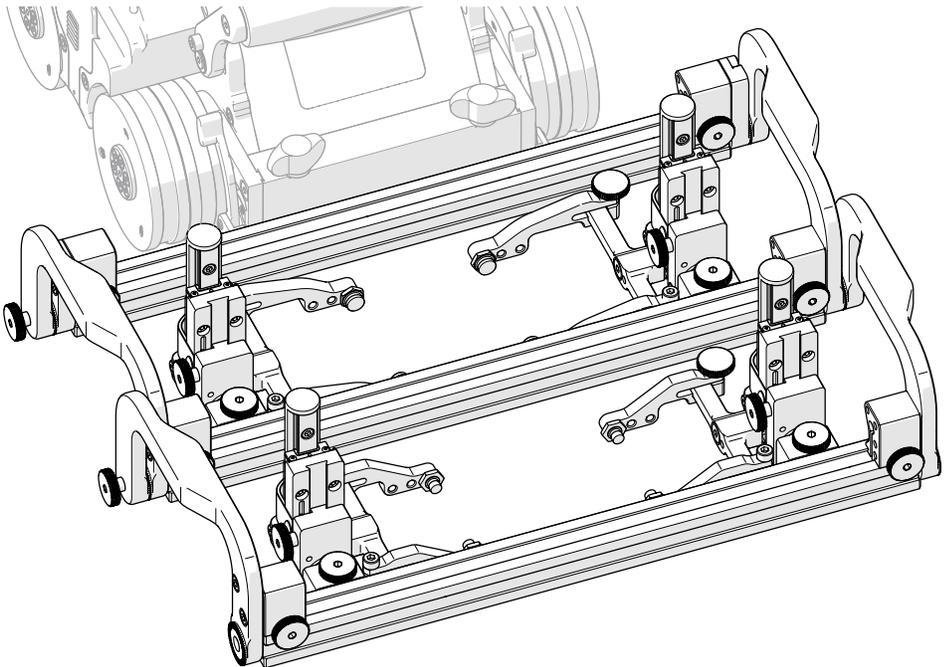


Fig. 177 - Vertical probe holder frame

1. Attach the wedges to the probe holders that will be used (*see Probe Holder Setup on page 60 for additional details*).

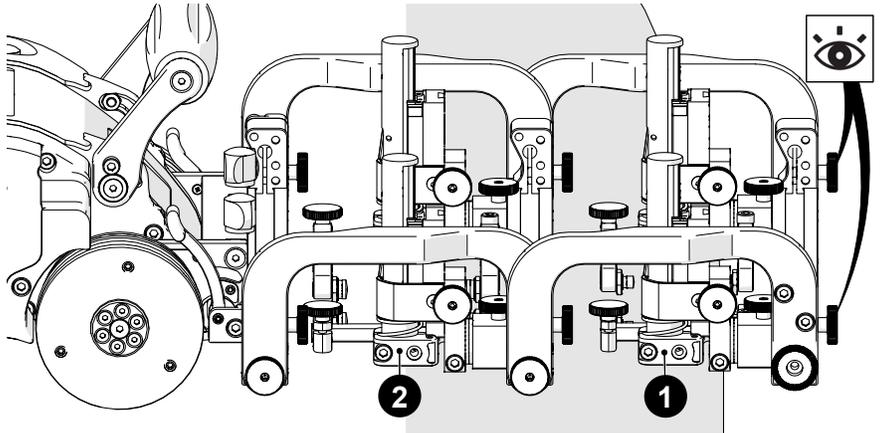


Fig. 178 - Position primary and secondary probe holders

2. Affix the probe holders (*with attached wedges*) to the probe holder frame. Place the secondary probe holder at the front of the frame (*Fig. 178-1*) and place the primary probe holders at the rear of the frame bar (*Fig. 178-2*).

TIP: Due to their larger size, scan results are generally improved when pulling or dragging phased array wedges.

3. Mount the probe holder frame to the crawler (*see Cable Retainer on page 51 for additional details*). When mounting the probe holder frame, ensure the attachment knobs (*Fig. 179*) are at the front (non crawler side).

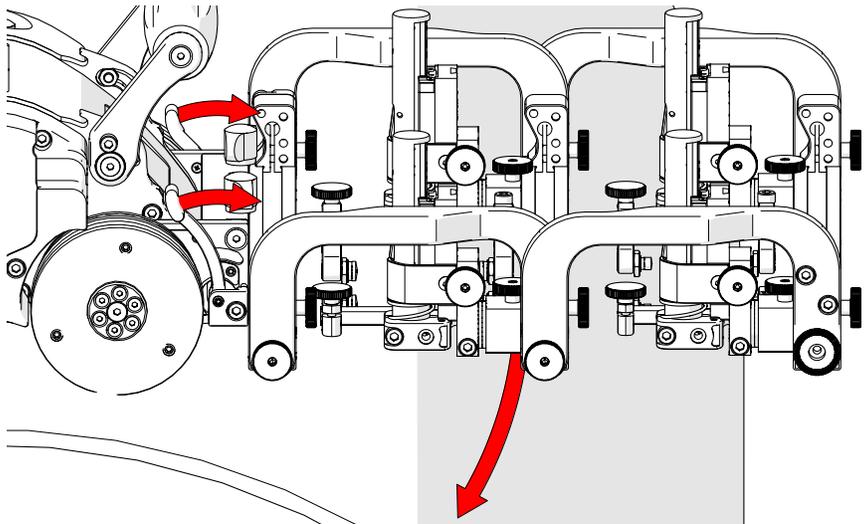


Fig. 179 - Align swivel mount with scan surface

4. Release the two swivel mount levers (Fig. 179) to position the swivel mount parallel to the scan surface (Fig. 180). When alignment with scan surface is achieved, lock the crawler swivel mount levers.

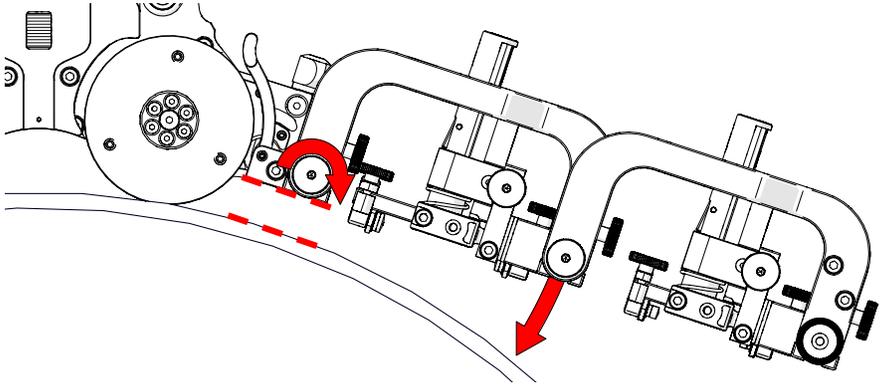


Fig. 180 - Set rear rotational adjustment knob

5. Loosen the rear rotational adjustment knob to lower the weld scan frame towards the inspection surface (Fig. 181).

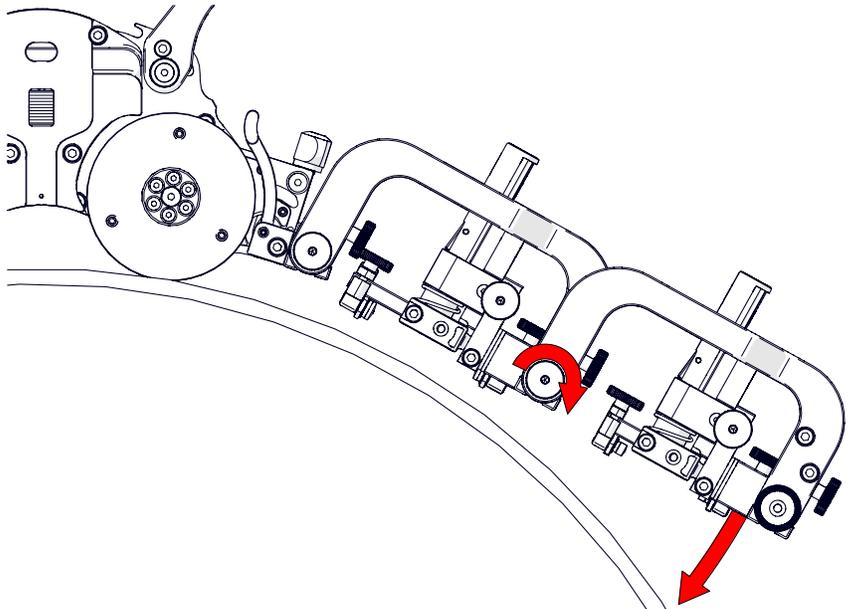


Fig. 181 - Set front rotational adjustment knob

6. Loosen the front rotational adjustment knob (Fig. 181) to align the TOFD probe holders parallel with the scan surface (Fig. 182).

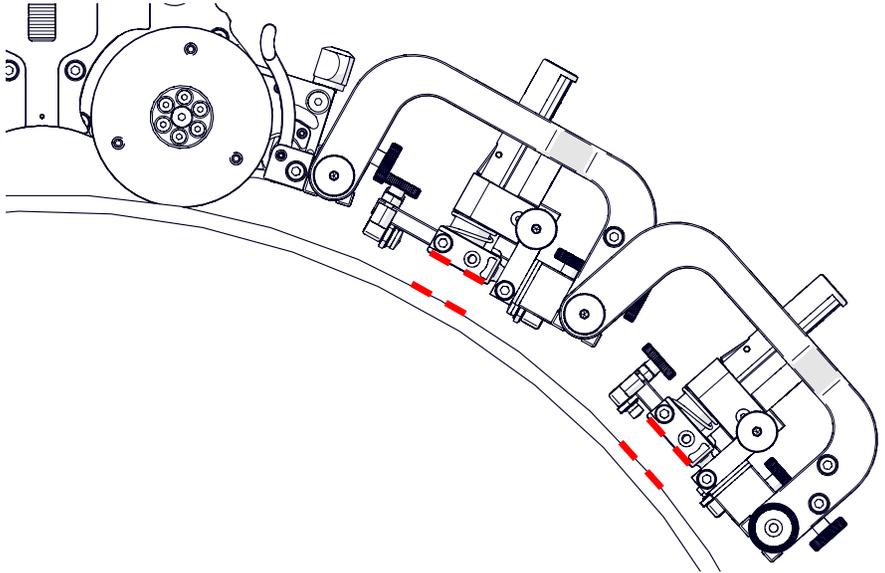


Fig. 182 - Align probes with the scan surface tangent

5.10.3. Pivoting Probe Holder Frame



WARNING! FALLING OBJECT HAZARD.

It is imperative that the steps below be followed to properly set the height of the probe holder frame. If the height of the probe holder frame is set too low, the crawler may fall and **SEVERE INJURY** or **DEATH** could result.

The pivoting probe holder frame utilizes vertical probe holders. The **SKOOT** can guide as many as six probes in the longitudinal direction.

NOTE: A minimum OD of 762 mm (30 in) is required for longitudinal scanning.

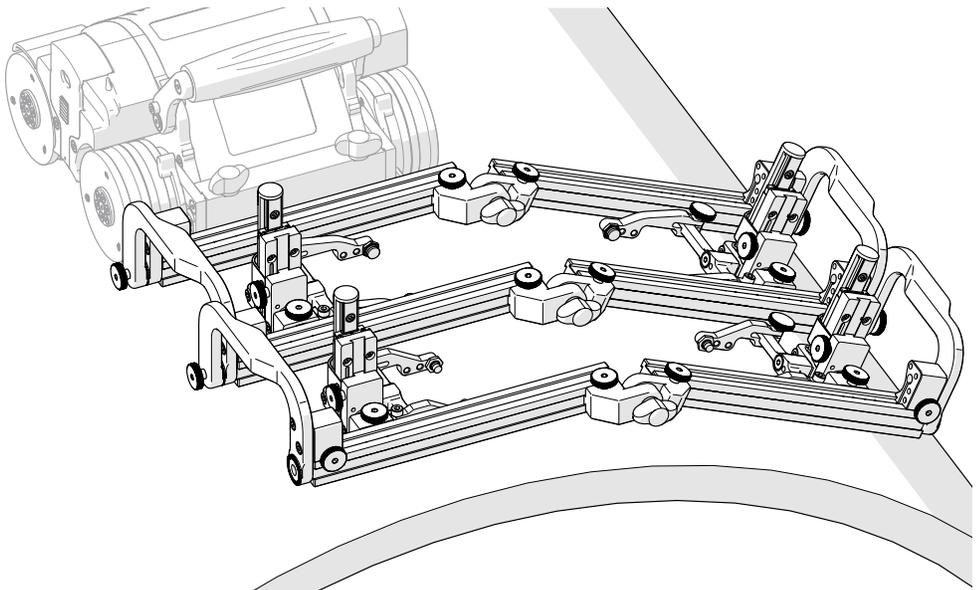


Fig. 183 - Pivoting Probe Holder Frame

5.10.3.1 Mounting a Pivoting Probe Holder Frame

1. If attached, use the 3 mm hex driver to remove the probe holder pivot mount from the pivoting probe holder frame.
2. Attach the wedges that are to be used with the probe holders (see *Probe Holder Setup* on page 60 for additional details).

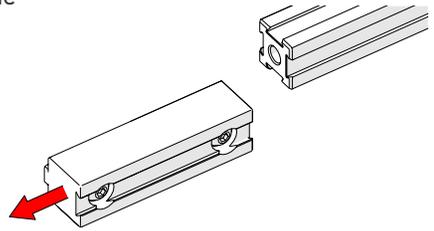


Fig. 184 - Remove probe holder pivot mount

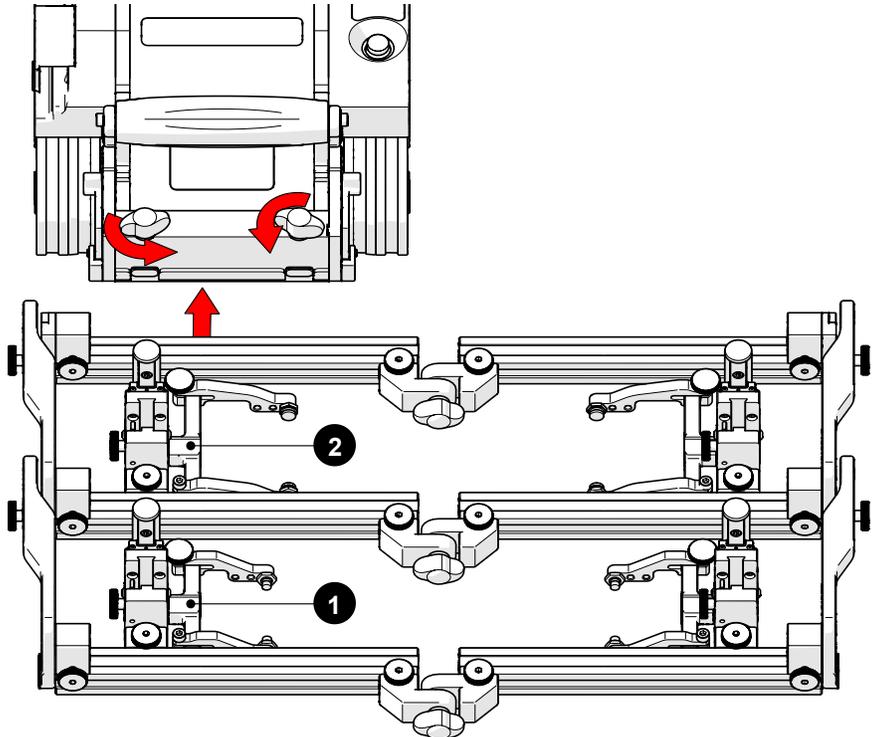


Fig. 185 - Connect frame to crawler's swivel mount

3. Affix the probe holders (*with attached wedges*) to the probe holder frame. Place the secondary probe holders at the front of the frame (Fig. 185-1) while placing the primary probe holders at the rear of the frame system (Fig. 185-2).

TIP: Phased array wedges are designed to be pulled along a scan surface.

4. Mount the pivoting probe holder frame to the crawler (see *Crawler* on page 48 for additional details).

5.10.4. Pivoting Probe Holder Frame Setup - Longitudinal Scanning

5.10.4.1 Longitudinal Scanning

To prepare the pivoting probe holder frame for longitudinal scanning, follow these steps:

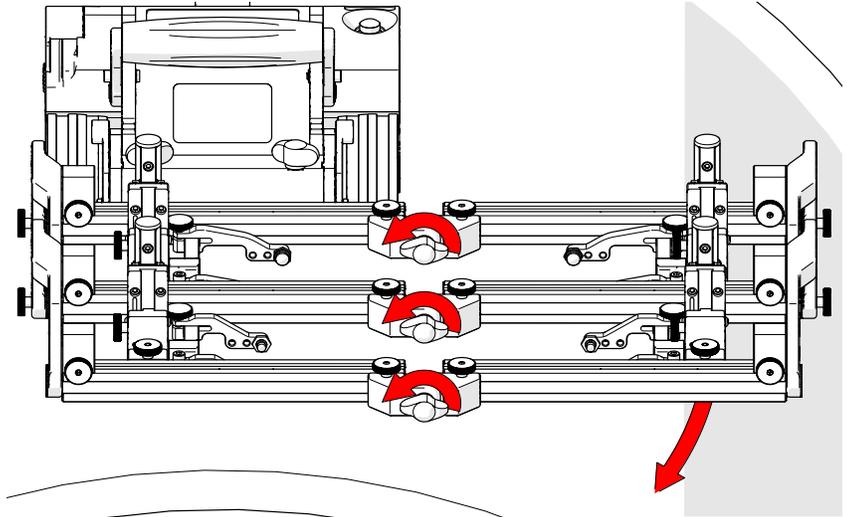


Fig. 186 - Loosen pivot wing knobs

NOTE: The swivel mount must be in a horizontal position during longitudinal scanning (see "Crawler" on page 48).

1. Loosen the pivot wing knobs at the centre of the frame system (Fig. 186). Lower the left side of the frame system to align with the tangent of the scan surface. Tighten the pivot wing knobs.

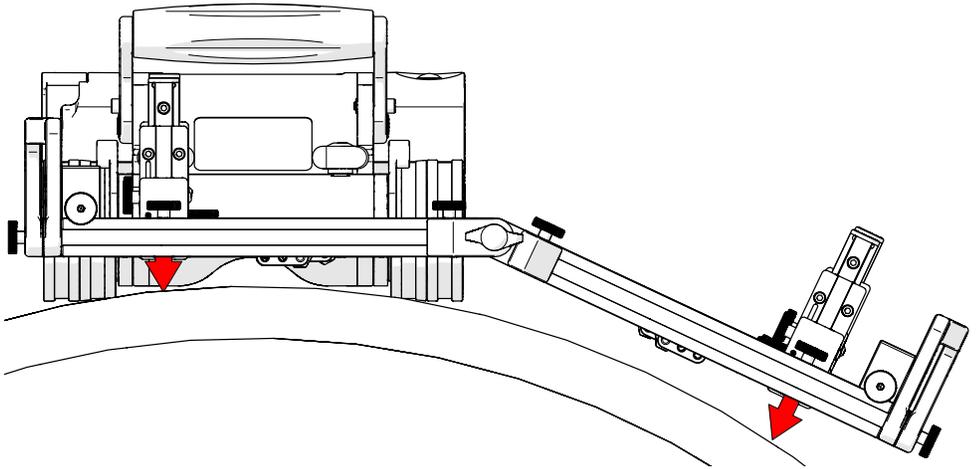


Fig. 187 - Tighten pivot wing knobs

2. Lower the vertical probe holders (see *"Probe Holder Vertical Adjustment"* on page 61).

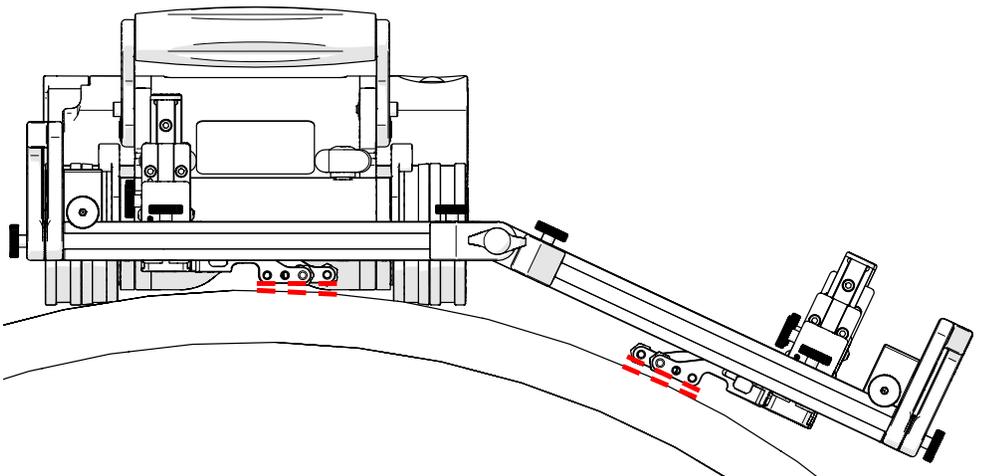


Fig. 188 - Correct probe holder longitudinal adjustment

3. Ensure probe holder arms are parallel to the scan surface (see *"Probe Holder Longitudinal Adjustment"* on page 63).

5.10.4.2 Circumferential Scanning

(see *Vertical Probe Holder Frame - Flat or Circumferential Only* on page 76 for additional details)

5.10.4.3 Pivoting Probe Holder Frame - Flange Scanning

NOTE: The optical guide pivot mount is not compatible with the following configuration.

The pivoting probe holder frame may be configured to allow scanning of flanges and the like. The following steps explain setup of this configuration:

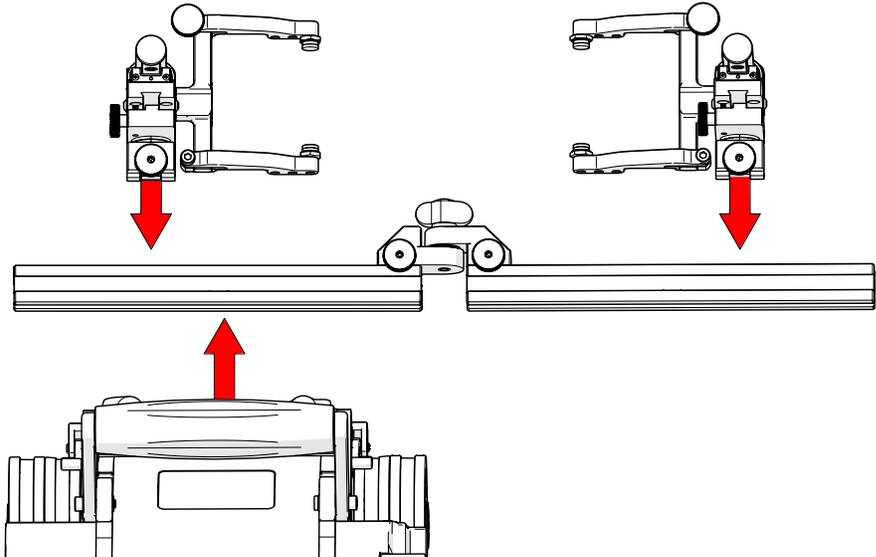


Fig. 189 - Configure assembly and mount to SK00T

1. Disassemble the pivoting probe holder frame to achieve the setup shown (Fig. 189). Ensure proper placement of the frame bar with attached mounting point in relation to the **SK00T**.

TIP: When the scanning surface is circumferential, only one frame bar with two probes can be used.

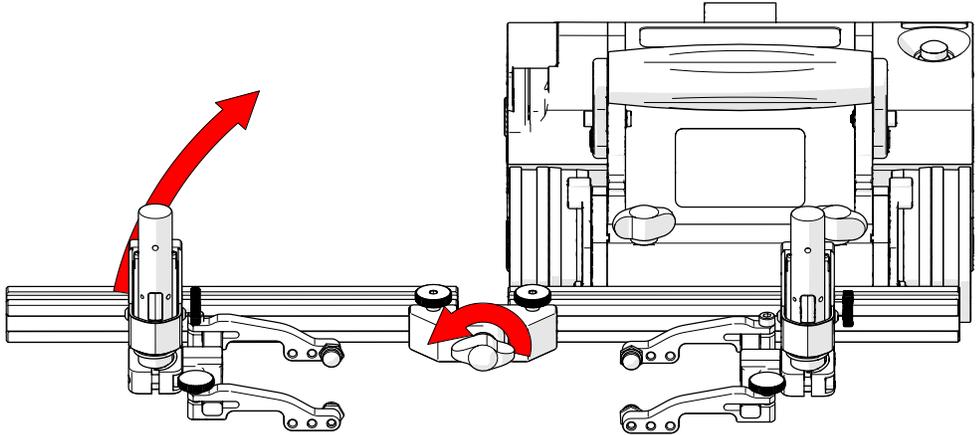


Fig. 190 - Lift frame bar to avoid interference

2. Loosen the pivot wing knob and raise the frame bar to an angle greater than the surface to be scanned (Fig. 190). Tighten the pivot wing knob and place crawler on scan surface (see "Placement of Crawler on Inspection Surface" on page 94)
3. Release the front swivel mount adjustment levers to align the swivel mount parallel to the scan surface (Fig. 191).

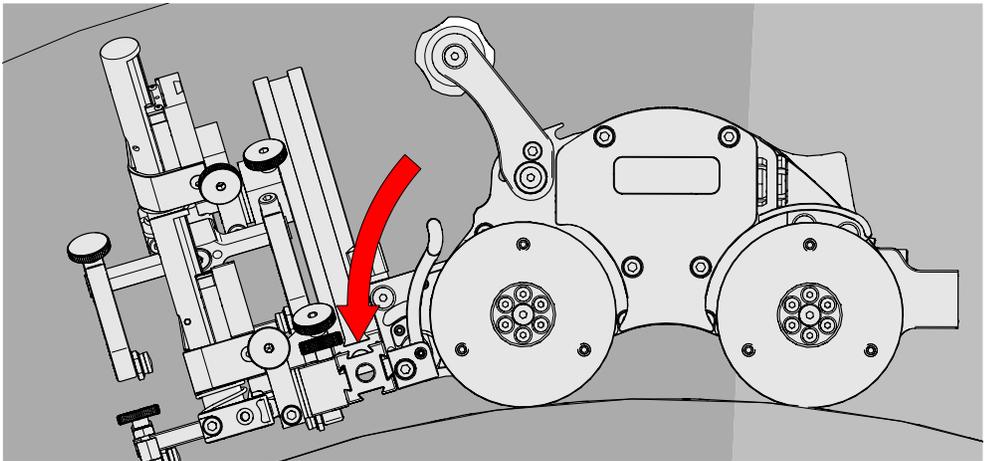


Fig. 191 - Align swivel mount with scan surface

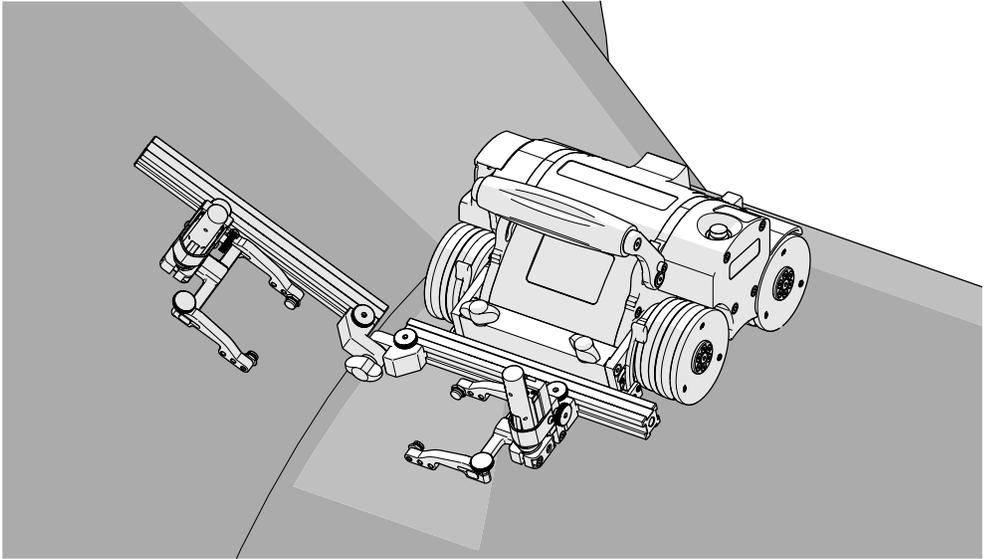


Fig. 192 - Align frame bar with flange scan surface

4. Loosen the pivot wing knob and align the frame bar parallel with the scan surface (*Fig. 192*).

5.10.5. Optical Guide Pivot Mount

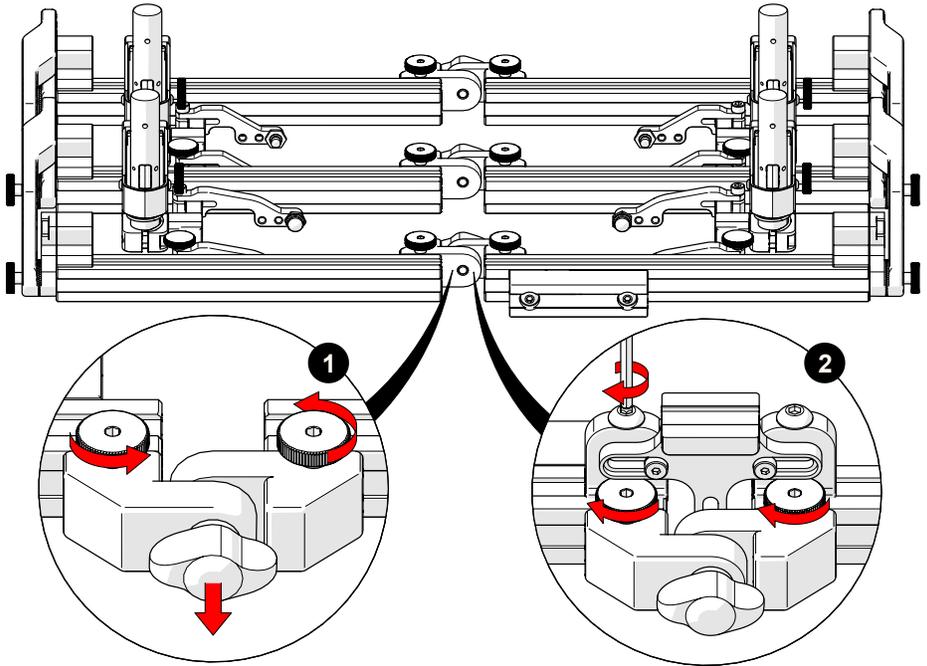


Fig. 193 - Correct probe holder longitudinal adjustment

An optional mounting point for any optical guide is available.

- ▶ (see “Battery Powered Optical Guide” on page 88)
- ▶ (see “Optical Guide” user manual)

To install the pivot mount, see these following instructions:

1. Remove the dovetail bar pivot from one of the sets of frame bars (*Fig. 193-1*). The choice of which dovetail bar pivot to remove is at the user’s discretion.
2. Attach the optical guide pivot mount to the frame bars (*Fig. 193-2*), tighten the dovetail knobs and the dovetail screws. Ensure a flush alignment of the pivot mount and the frame bars to achieve proper centering of the optical guide pivot mount.
3. Mount an optical guide see the appropriate instructions listed above.

5.11. Accessories

5.11.1. Battery Powered Optical Guide



WARNING! LASER RADIATION. Do not view directly with optical instruments. Class 1M laser product.

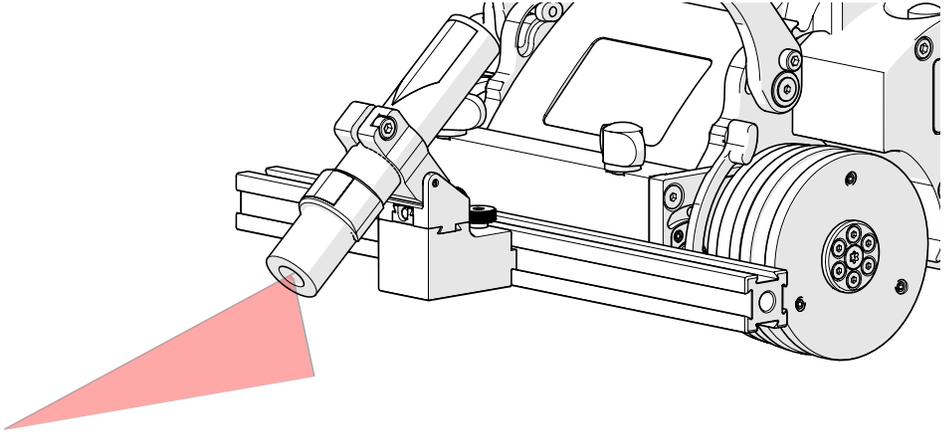


Fig. 194 - Battery powered optical guide

The battery powered optical guide provides a reference point useful for aligning the **SKOOT** to a given path (*i.e.* a weld). The battery powered optical guide may be installed and setup as follows:

1. Loosen the optical guide knob.
2. Mount the optical guide to the frame bar, tighten the optical guide knob (Fig. 195).
3. Adjust the optical guide's friction pivot aiming the beam at the inspection surface (Fig. 196).
4. Loosen the optical guide knob to adjust the side-to-side position as required. Retighten the optical guide knob.

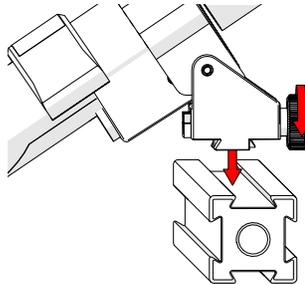


Fig. 195 - Mount on frame bar

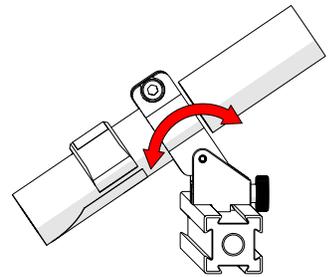


Fig. 196 - Aim guide

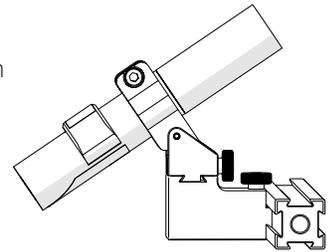


Fig. 197 - Perpendicular mount

NOTE: The battery powered optical guide requires 1 AA battery for operation.

5.11.2. Cable Management

The cable management is offered in a variety of lengths and provides a means of bundling and protecting cables and hoses that connect to the scanner.

5.11.2.1 Mounting the Cable Management

To attach cable management with threaded mount, follow these steps:

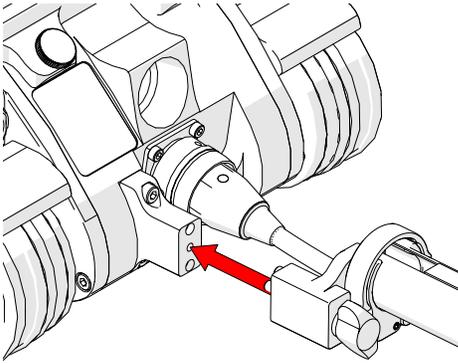


Fig. 198 - Align with umbilical

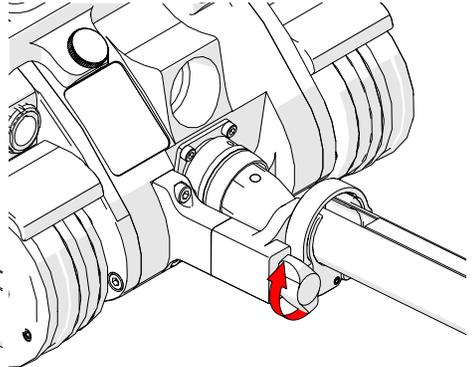


Fig. 199 - Tighten wing knob

1. Align the cable management clamp with the appropriate mounting position on the user umbilical breakout (Fig. 198).
2. Tighten the cable management clamp wing knob (Fig. 199).

5.11.2.2 Cable Management Setup

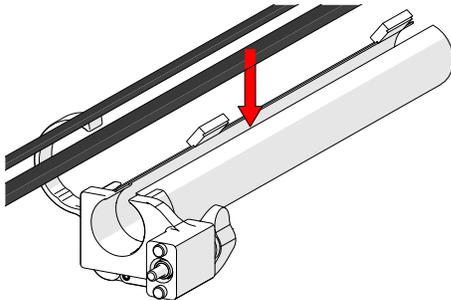


Fig. 200 - Insert cables and hoses

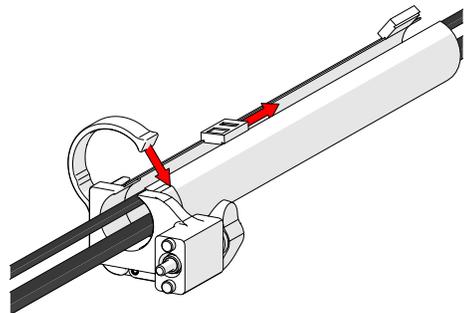


Fig. 201 - Zip to close

1. Open the cable management. Begin at the clamp end and start placing the cabling in the tube (Fig. 200).
2. Follow the cable placement zipping the tube closed (Fig. 201).

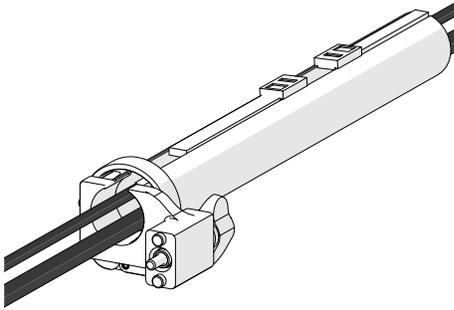


Fig. 202 - Zip opposite end

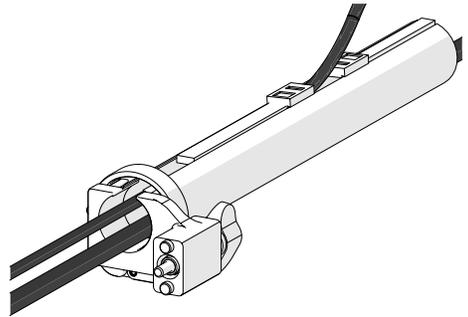


Fig. 203 - Flexible routing

3. Once the cable is placed the entire length of tube, bring the zipper from the opposite end to meet at any point in the middle.

When necessary, the two zippers may be opened to allow any cables to be routed out of the tube.

5.11.2.3 Clamp Setup

In the event the tube becomes disconnected from the cable management clamp, follow these instructions to reattach the tube and clamp.

Loosen the clamp screw using the supplied 3 mm hex driver. Slide the clamp around the tube first and then slide the tube around the outside of the cable management mount (Fig. 204). Align the zipper opening and the cable management clamp opening.

Slide the clamp over the tube and cable management mount pinching the tube in between (Fig. 205).

Tighten the clamp screw (Fig. 206).

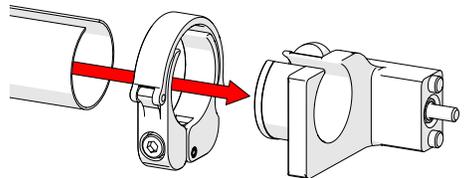


Fig. 204 - Slide tube around mount

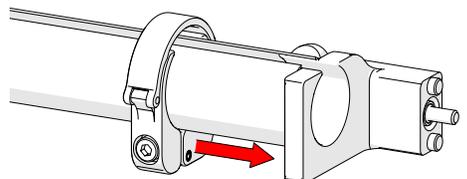


Fig. 205 - Slide clamp onto mount

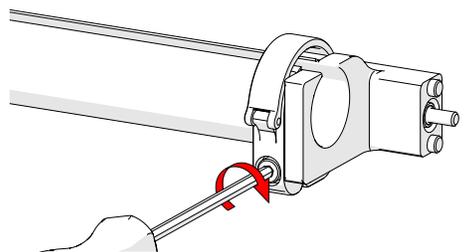


Fig. 206 - Tighten clamp screw

5.11.3. Preamp Bracket

Intended Use:

- ▶ The **SKOOT** preamp bracket is intended to mount objects (eg. preamps, splitters, etc) that:
- ▶ have a maximum weight of 1.36 kg (3 lb)
- ▶ are attached to the **SKOOT** with a lanyard or probe cables strong enough to prevent the object from falling
- ▶ have smooth edges so as not to cut preamp velcro strap

To install and use the preamp, follow these steps:

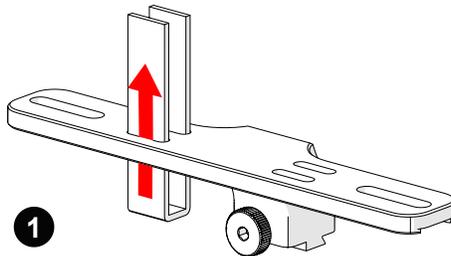


Fig. 207 - Insert Velcro straps

The preamp bracket mounts to any dovetail groove to hold a preamp. Compatible with most standard preamps, use the adjustable screw mounting channel on the bottom of the bracket to attach a preamp. The preamp bracket may also be ordered with Velcro straps which are used to hold the preamp.

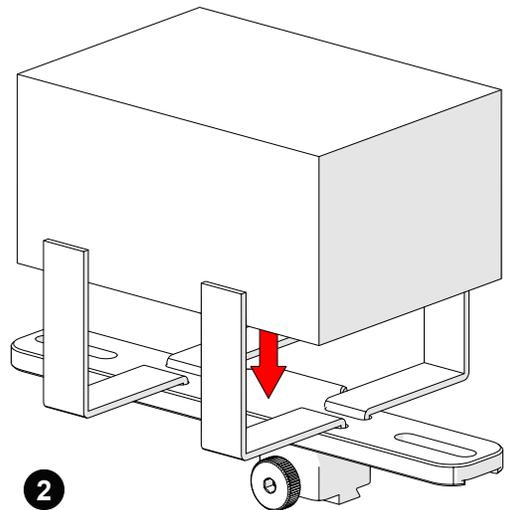


Fig. 208 - Place preamp and wrap velcro

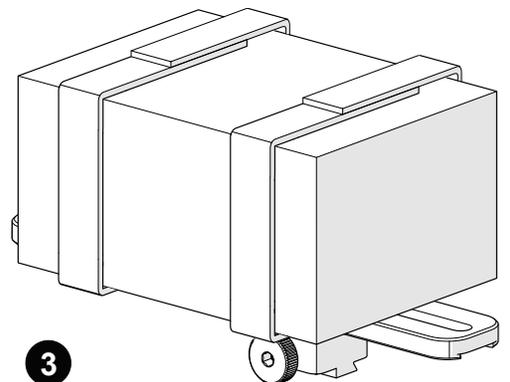


Fig. 209 - Mount bracket on a frame bar

OPERATION

6.1. System Startup

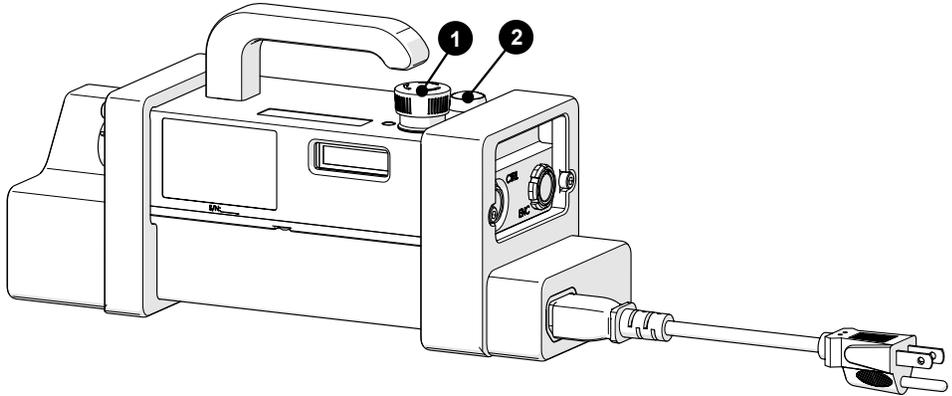


Fig. 210 - Power controller

To activate the system, follow these steps:

1. Plug-in the power controller to the appropriate power source (see “Power Requirements” on page 10).
2. Connect the components (see “Configurations” on page 40)
3. Locate the red emergency stop push-button (Fig. 210-1) on the power controller. Rotate this button clockwise to unlatch.
4. The green push-button (Fig. 210-2) on the power controller activates the system.



Fig. 211 - Handheld controller

5. A warning message will display on the handheld controller when power has been activated (*Fig. 211*). Once the dangers of using the **SKOOT** are recognized and understood by reading this user manual, touch **Ok** to acknowledge the warning.



Fig. 212 - Falling object warning

6. A second warning message (*Fig. 212*) will display requesting assurance that a No Entry Fall Zone has been established (*see "Preparation for Safe Use" on page 35*) and tether requirements are met (*see "Tether Requirements and Attachment" on page 36*). Acknowledge this warning by touching **Yes**.

Once the system is initialized, the **Mode Select** screen will appear (*see "Mode Select Screen" on page 98*). The system is now ready for operation.

6.2. Placement of Crawler on Inspection Surface



WARNING! FALLING OBJECT HAZARD.

Read and understand the proper procedure for using the Installation/Removal Mat. If crawler installation is done at elevated heights, improper use may cause the crawler to fall and **SEVERE INJURY** or **DEATH** could result.



CAUTION! Do **NOT** handle crawler using the umbilical cable. Use the provided handle.



CAUTION! To place the crawler on the inspection surface, use the scanner installation/removal mat (*Fig. 56*) as a spacer between the wheels and the surface on which the crawler is to drive. This is necessary to protect the electronic components within the crawler from damaging shock, should the crawler be slammed directly onto the surface.



WARNING! MAGNETIC MATERIAL. The wheels of the crawler produce an extremely strong magnetic field which may cause failure or permanent damage to items such as watches, memory devices, CRT monitors, medical devices or other electronics.



Tools, magnets and metal objects can cut, pinch or entrap hands and fingers. **HANDLE WITH CARE.**

People with pacemakers or ICD's must stay at least 75 cm (30 in) away.

WARNING! MAGNETIC MATERIAL. The installation/removal mat contains magnetic material. Those with pacemakers or ICD's must stay at least 10 cm (4 in) away.

6.2.1. Scanner Installation/Removal Mat Use

To place the crawler on the inspection surface, follow these steps:

NOTE: For scanner installation/removal on inspection surfaces with a temperature between 50°C and 150°C (122°C and 302°C), use the medium temperature installation/removal mat found in the automated crawler medium temperature add-on kit. Also, ensure the medium temperature cable management is used in place of cable management (see “Cable Management” on page 89)

NOTE: The manufacturer recommends two persons install the crawler on an inspection surface. One person to lower the crawler to the scan surface and one person to operate the crawler via the handheld controller.

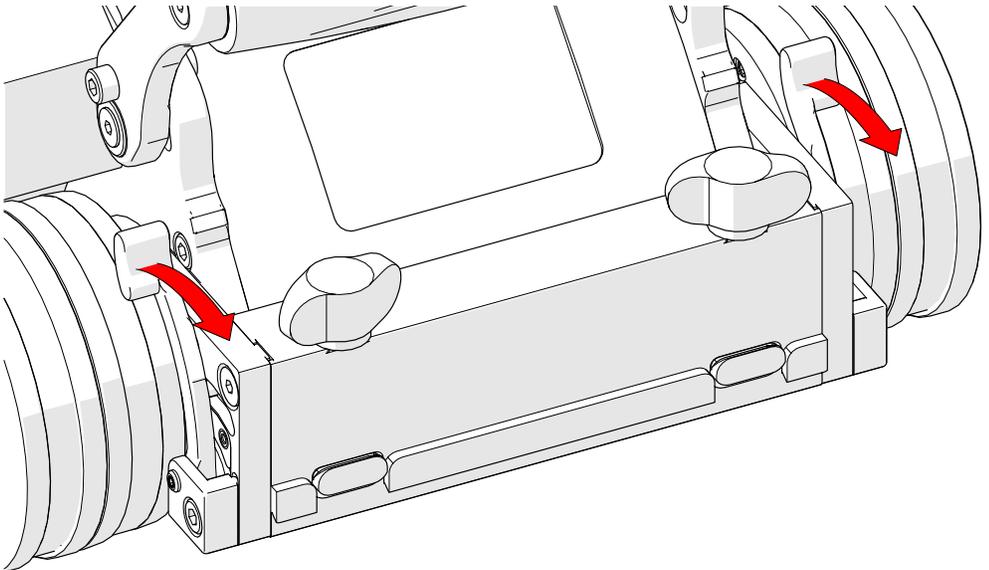


Fig. 213 - Front swivel adjustment levers

1. Once crawler preparation is complete (see “System components” on page 20) and system startup has been performed (see “System Startup” on page 92), raise the front swivel mounts to ensure they will not hinder the wheels from contacting the inspection surface (see “Crawler” on page 48). Release the front swivel adjustment levers (Fig. 213), located at the front of the crawler, to position the front swivel mount.
2. Set the crawler to Jog Mode (see “Jog Mode” on page 99).

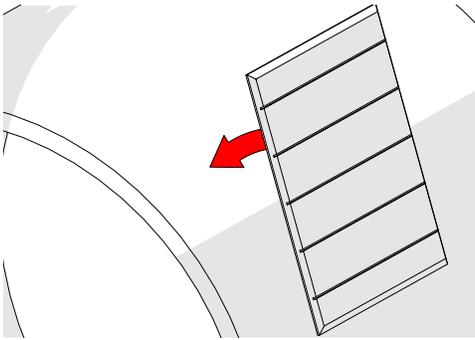


Fig. 214 - Place installation/removal mat

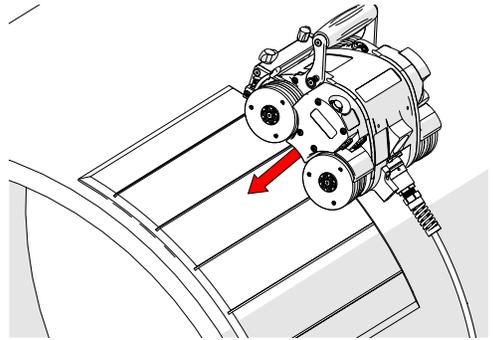


Fig. 215 - Lower crawler to mat

3. Place the installation/removal mat (Fig. 14) on the inspection surface (Fig. 214).
4. Place and hold the crawler on the installation/removal mat (Fig. 215).

NOTE: Do **NOT** release crawler when placed on the installation/removal mat.

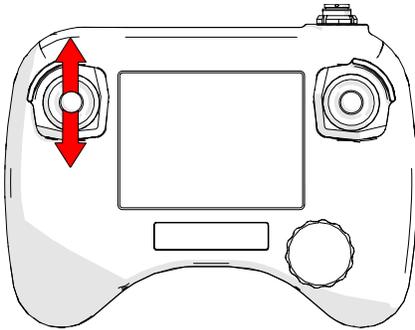


Fig. 216 - Drive the crawler

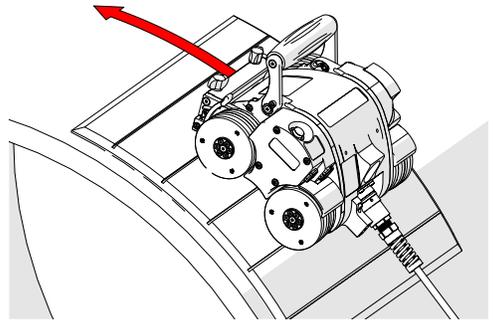


Fig. 217 - Drive crawler off the mat

5. Ensure all four wheels of the crawler are held firmly against the installation/removal mat. While holding the crawler, use the Fwd/Rev joystick (Fig. 216) to carefully drive the crawler (Fig. 217) off the installation/removal mat and onto the inspection surface (Fig. 218).

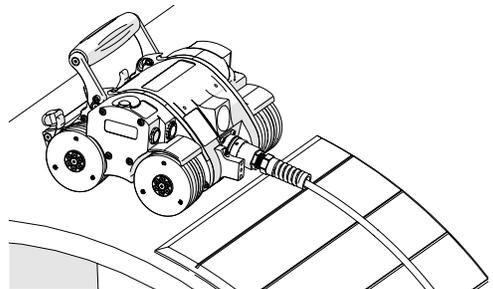


Fig. 218 - Magnetized to surface

TIP: Avoid the crawler slamming to the inspection surface. This can occur when all four wheels are not in contact with the installation/removal mat while the crawler is driven onto the inspection surface.

6. Remove the installation/removal mat from the inspection surface.

TIP: Circumstance may arise when only one person is available for placement of the crawler on a inspection surface. With the system power off, it is possible to place the crawler on the inspection/removal mat and manually push the crawler off the mat and onto the inspection surface.

6.3. Operation

6.3.1. Handheld Controller Layout

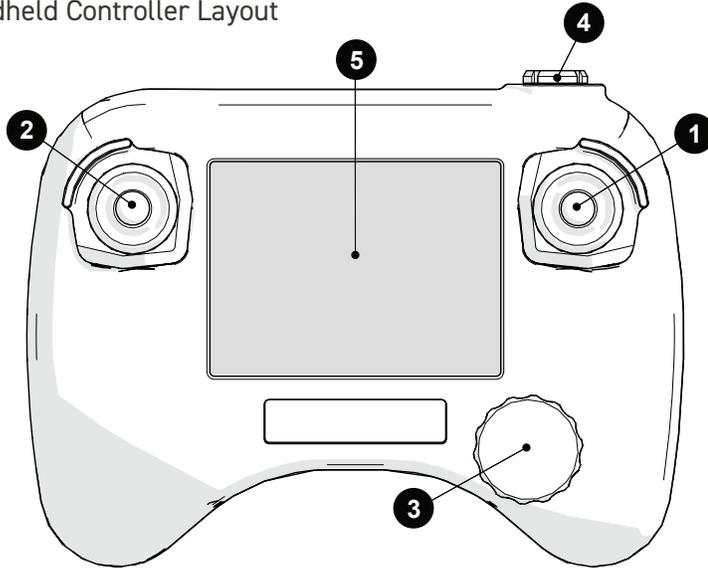


Fig. 219 - Handheld controller

1	Raster joystick	(see "Joysticks" on page 98)
2	Fwd/Rev joystick	(see "Joysticks" on page 98)
3	Click wheel	(see "Click Wheel" on page 98)
4	Controller cable connector	Connection point for the auxiliary cable.
5	Touchscreen	(see "Touchscreen" on page 97)

6.3.1.1 Touchscreen

The handheld controller touchscreen (Fig. 219-5) is the primary operator interface for the system. Buttons are indicated on-screen with a 3D border (Fig. 220).



Fig. 220 - Sample touchscreen buttons

6.3.1.2 Click Wheel

The click wheel (Fig. 219-3) provides a redundant system control that may be utilized in lieu of the touchscreen. A blinking box around a button indicates the click wheel selection. Rotating the click wheel selects different buttons on-screen. Press the click wheel to choose the button currently selected.

6.3.1.3 Joysticks

The joysticks are used to control the system. The left joystick (Fig. 219-2) controls the forward/reverse movement of the crawler. The right joystick (Fig. 219-1) controls raster arm movement.

6.3.2. Mode Select Screen

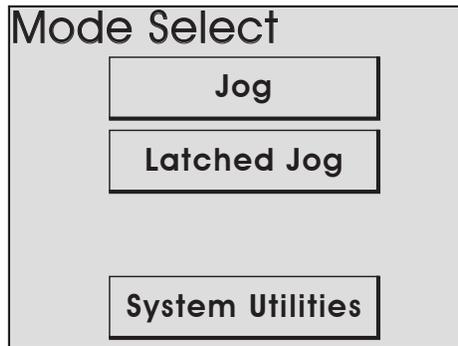


Fig. 221 - Mode select

The **Mode Select** screen offers four modes of operation for the system:

Jog Mode	(see "Jog Mode" on page 99)
Latched Jog Mode	(see "Latched Jog Mode" on page 101)
System Utilities	(see "System Utilities Screen" on page 102)

6.3.3. Jog Mode

Jog mode manually controls the system movement using the joysticks.

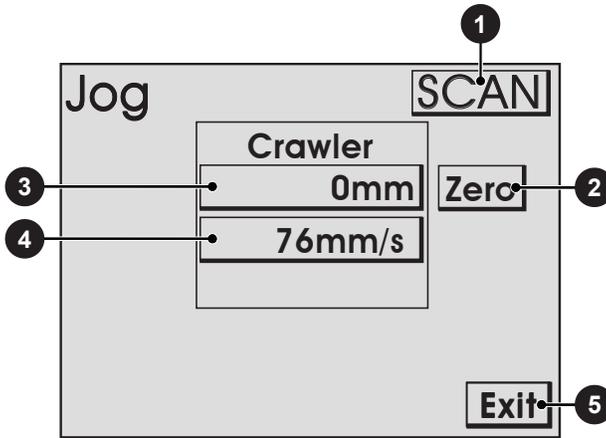


Fig. 222 - Jog mode

Jog mode manually controls the system movement using the joysticks.

- 1 Scan/Rapid Button (Fig. 222)

Used to quickly switch between crawler speeds. The speed in either mode can be manually set to the users preference.

***TIP:** Fine adjustments of speed can be made in the User Settings (see "User Settings Screen" on page 102).*

- 2 Zero Button (Fig. 222)

Sets the current position to zero for all modules.

- 3 Module Position Button(s) (Fig. 222)

Displays the current position of the crawler. Press to set the position to any value using the **Edit** screen. When a module position is modified, the position will be modified for all other system modes.

***NOTE:** This function only zeroes the number displayed on the **SKOOT** handheld controller. It does not zero the position used in the data acquisition instrument.*

- 4

 Module Rate Button(s)
(Fig. 222)

 Displays the current maximum rate for the selected speed mode. Press to set the maximum rate using the **Edit** screen. The movement commanded by the joysticks will be limited to the indicated rate. When a rate is modified, the rate will be modified for all other system modes.
- 5

 Exit Button: *(Fig. 222)*

 Exits the jog mode and returns to the **Mode Select** screen.
- 6

 BiasOn/BiasOff button
(Fig. 222)

 When the Steering Bias setting is non-zero, this button will be displayed to allow the set steering bias for the right steering joystick to be turned on and off.

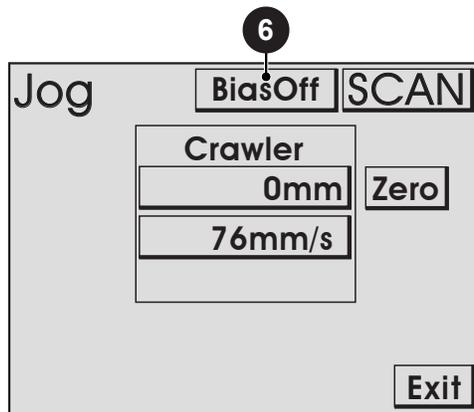


Fig. 223 - BiasOn/BiasOff button identification

6.3.4. Latched Jog Mode

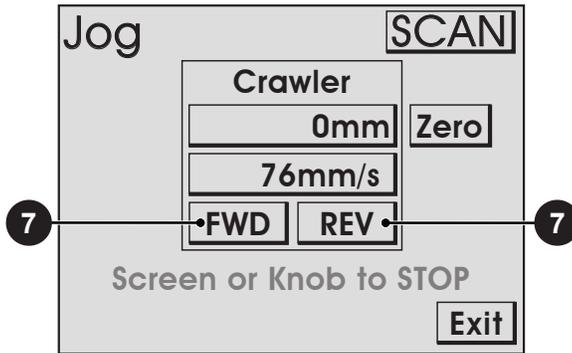


Fig. 224 - Latched jog mode

Identical to standard jog mode, latched jog mode adds forward or reverse crawler movement at the selected scan rate. This eliminates the need to manually hold the left joystick (see “Jog Mode” on page 99).

7 FWD & REV Buttons:

The **FWD** and **REV** buttons are located in the crawler tab. Press the **FWD** or **REV** button to drive the crawler at the current maximum scan rate. Touching the handheld controller screen or pressing the click wheel stops crawler movement.

NOTE: The *FWD & REV Buttons will not be present in rapid mode.*

6.3.5. System Utilities Screen

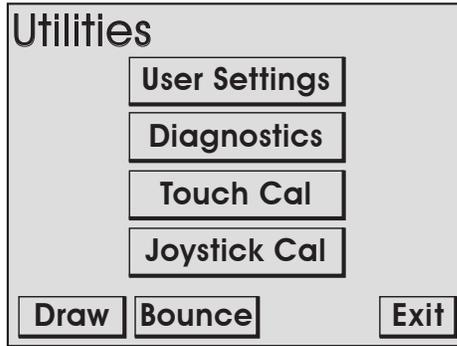


Fig. 225 - Utilities screen

The **Utilities** screen provides access to the setup, diagnostics and user preference settings.

<p>User Settings Button (Fig. 225)</p>	<p>Access the User Settings screen allowing for various user preferences to be adjusted.</p>
<p>Diagnostics Button (Fig. 225)</p>	<p>Enters the Diagnostic screens which may be used to monitor system components and function.</p>
<p>Touch Cal Button (Fig. 225)</p>	<p>Used to initiate the Touch Calibration screen.</p>
<p>Joystick Cal Button (Fig. 225)</p>	<p>Used to enter the Joystick Calibration screen.</p>
<p>Draw Button (Fig. 225)</p>	<p>Enters mode used to test the touch screen accuracy and response</p>

6.3.5.1 User Settings Screen

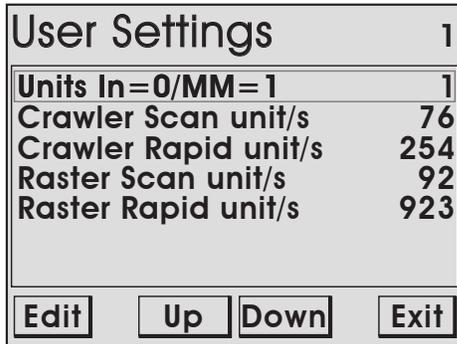


Fig. 226 - User settings screen

Allows user to customize the system to their preferences.

The blinking highlighted box indicates the current selection. Use the click

knob or **Up** and Down buttons to select different settings.

Press **Edit** to enter the **Edit** screen to apply changes to the selected setting.

The **Exit** button direct to the **System Utilities** screen.

TITLE	DESCRIPTION	VALID RANGE	DEFAULT
Units In=0/MM=1	Changes the measurement units for display and user entry. When set to 0, units measure in inches. When set to 1, units measure in millimeters.	0-1	1
Crawler Scan unit/s	Sets the crawler scan rate in the current units/second. This setting can also be changed through the Jog or Two Axis Scan Speed screens	5-142 mm/s (0.2-5.6 in/s)	43 mm/s (1.7 in/s)
Crawler Rapid unit/s	Sets the crawler rapid rate in the current units/second. This setting can also be changed through the Jog screen.	5-142 mm/s (0.2-5.6 in/s)	142 mm/s (5.6 in/s)
Raster Scan unit/s	Sets the raster arm scan rate in the current units/second. This setting can also be changed through the Jog or Two-Axis Scan Speed screens.	5-762 mm/s (0.2-30 in/s)	76 mm/s (3.0 in/s)
Raster Rapid unit/s	Sets the raster arm rapid rate in the current units/second. This setting can also be changed through the Jog screen.	5-762 mm/s (0.2-30 in/s)	762 mm/s (30.0 in/s)
*Raster Flip 0/1	Set raster arm orientation. When the raster arm is mounted with the motor housing to the left of the crawler, the appropriate setting is 1. When the raster arm is mounted with the motor housing to the right of the crawler, the appropriate setting is 0. When this setting is changed, the system must be rebooted.	0-1	1

6.3.5.2 Diagnostics Screens

Several diagnostic screens allow various system functions to be monitored. Navigate to different diagnostic screens using the **PREV** and **NEXT** buttons. The **Exit** button returns to the **System Utilities** screen.

NOTE: *The diagnostic information requires an in depth understanding of the underlying technologies and programming in the system. Not all functions and information is explained in this manual.*

6.3.5.2.1. Detected Modules

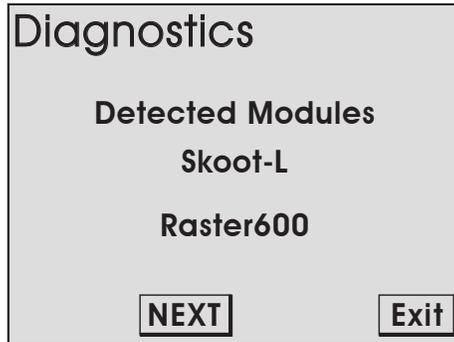


Fig. 227 - Detected modules screen

Screen indicates the system software version and displays which modules were detected when the system was activated.

6.3.5.2.2. System 1

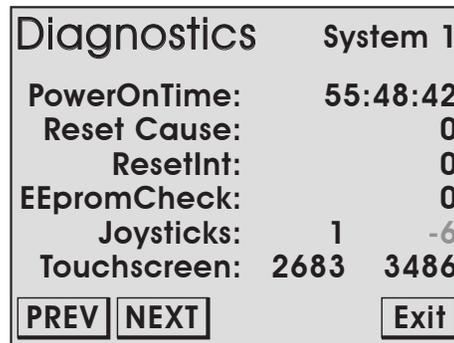


Fig. 228 - Diagnostic screen

System 1 diagnostic screen displays general system function information.

PowerOnTime	The total accumulative time the handheld controller has been powered
Joysticks	Indicates the raw position reading from the joysticks
TouchScreen	Indicates the raw position reading from the last touchscreen contact

6.3.5.2.3. System 2

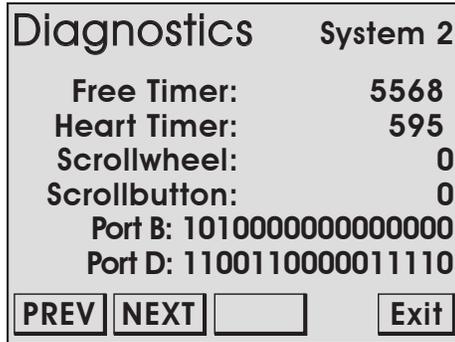


Fig. 229 - Diagnostic screen

Additional general system function information is displayed within the **System 2** screen. An empty button is provided to allow testing of the click wheel.

Free Timer	Value from a free running system timer. If this timer is static, an internal controller issue is present
Scrollwheel	Counter indicating the rotary position of the click wheel.
Scrollbutton	Indicates the status of pressing the click wheel

6.3.5.2.4. System 3

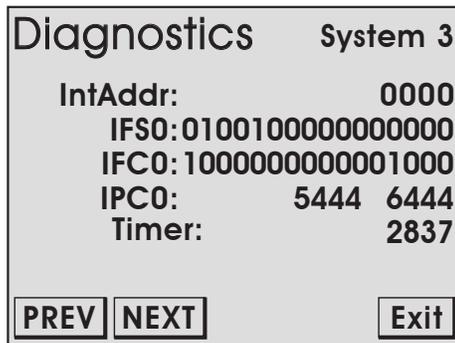


Fig. 230 - Diagnostic screen

The **System 3 Diagnostic** screen displays additional system information. The information provided does not typically assist the user.

6.3.5.2.5. Skoot-L, Raster

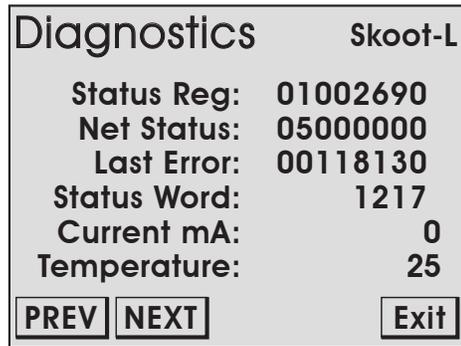


Fig. 231 - Diagnostic screen

The **Skoot-L diagnostic** screen provides information regarding the status of the crawler. A separate screen is available for each module detected upon system startup.

Current MA

Displays the output of the crawler to the motor. The current (mA) displayed is directly proportional to the motor's output torque. This reading can be used to check if the control system is responding to forces on the modules motor

Temperature

Internal temperature reading of the crawler in degrees Celsius

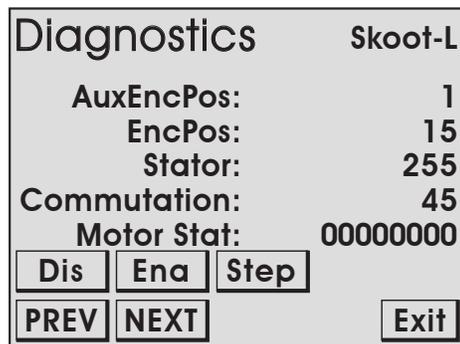


Fig. 232 - Diagnostic screen

AuxEncPos	Displays the position of the auxiliary encoder in counts when connected to the module. When the auxiliary encoder is moved, this number will change. When the encoder is moved from its current position and then back to that exact same position, this number will also return to its original position
EncPos	The position of the modules motor encoder in counts

6.3.5.3 Touch Calibration Screen



Fig. 233 - Touch calibration screen

This option allows calibration of the touch screen. Typically, this should not be necessary.

Touch the screen as the markers appear in the four corners of the screen.

***TIP:** It is recommended that the markers be touched with a small object to enhance the touch position accuracy during calibration.*

The new calibration is stored immediately when the fourth marker is pressed. The calibration utility exits and return to the **System Utilities** screen. To abort the calibration, the system power may be turned off before the last marker is pressed.

6.3.5.4 Joystick Calibration Screen

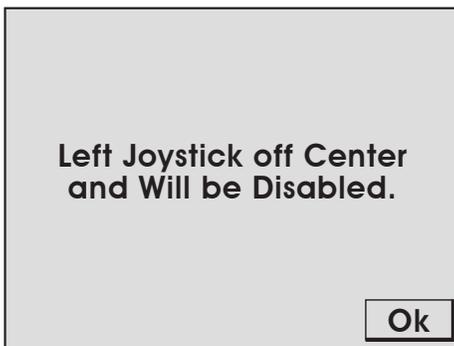


Fig. 234 - Joystick error

Typically joystick calibration is only necessary when a joystick off center error is detected upon startup (*Fig. 234*). Calibration may also be used when a joystick function does not appear to be properly centred.

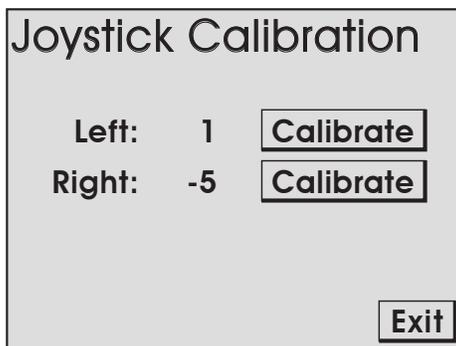


Fig. 235 - Joystick calibration screen

Current readings of the joysticks are displayed in the **Joystick Calibration** screen (*Fig. 235*). When the numbers are not near zero, press the **Calibrate** button to recalibrate to 0. The new calibration is stored when the **Exit** button is pressed.

6.3.5.5 Draw



Fig. 236 - Draw utility

The draw utility may be used to test the function of the touchscreen. Exit the utility by pressing the click wheel.

6.3.6. High Internal Temperature Screen



CAUTION! HOT SURFACE. The handles of the crawler and crawler body may be hot to the touch. Use appropriate protective equipment when removing a crawler from a high temperature surface.



Fig. 237 - High internal temperature screen

When the system approaches its maximum operating temperature, the high internal temperature screen will display. When this alert screen is displayed, all motor and system function will cease.

Press **OK** to reactivate the system to remove **SKOOT** from the scan surface.

MAINTENANCE

7.1. Safety Precautions Before Maintenance



WARNING! ELECTRICAL SHOCK

HAZARD. Disconnect the power controller when servicing the equipment. The power controller is powered even when the E-Stop push-button is latched in the off position.



WARNING! MAGNETIC MATERIAL.

The wheels of the crawler produce an extremely strong magnetic field which may cause failure or permanent damage to items such as watches, memory devices, CRT monitors, medical devices or other electronics.

Tools, magnets and metal objects can cut, pinch or entrap hands and fingers. **HANDLE WITH CARE.**

Those with pacemakers or ICD's must stay at least 25 cm (10 in) away at all times.

7.2. Cleaning

General cleaning of all components is important to keep the system working properly. All components that do not have wiring or cables are completely waterproof.

Components can be washed with warm water, dish soap and a medium bristle brush.

Before using the scanner ensure that all connectors are free of water and moisture.

TIP: All components with wiring, cables or electrical connections are splash proof but not submersible.

NOTE: Never use strong solvents or abrasive materials to clean your scanner components.

7.3. Maintenance Schedule

The **SKOOT** system must be maintained according to the following schedule.

Task	Frequency
<u>Inspect safety apparatus</u>	
This includes:	
<ul style="list-style-type: none">● All components of tether system. Replace damaged components as necessary.● Lifting sling on crawler. If the lifting sling shows signs of damage (<i>e.g. cuts, abrasion, etc</i>) do NOT use.	Every Use
<u>Clean the drive wheels</u>	
Debris will collect on the magnetic wheels. Remove this debris before every use. An effective cleaning method uses adhesive-backed tape (<i>e.g. duct tape</i>) to 'pull' the debris off the wheels.	Every Use
<u>Inspect cables and connectors</u>	
Inspect the umbilical cable, the control cable and the power controller cable for damage. Have any damaged cable repaired by a qualified person or replace the cable assembly as necessary.	Every Use
Inspect all connectors for damage or moisture. Straighten bent pins. Dry connectors before using.	
<u>General cleaning</u>	
Ensure that the scanner stays relatively clean by wiping off any excess dirt or other contaminants after every use.	Every Use

TROUBLESHOOTING

8.1. Startup Issues

Two messages are possible in the event of a startup issue: **Joystick Off Center** or **Checking Network**.

8.1.1. Joystick Off Center

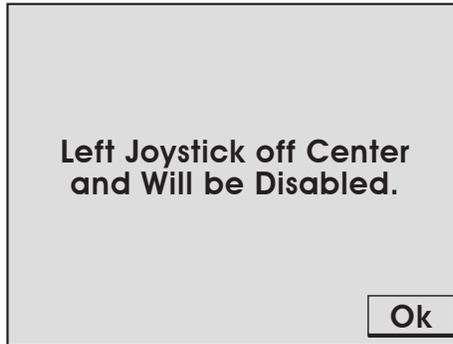


Fig. 238 - Joystick off centre screen

Upon system startup, the joystick positions are detected. When a joystick is detected outside the centre position, the **Joystick Off Center** screen displays indicating the joystick will be disabled. Press **Ok** to continue system startup. All system functions will work normally with the exception of movements that require joystick operation.

Ensure the handheld controller's joysticks are free of interference and reset the system power to enable joystick control.

If no interference of the joystick is present, the joystick calibration may need to be performed (see "Joystick Calibration Screen" on page 109)

8.1.2. Checking Network



Fig. 239 - Checking network screen

During startup, the system initializes the communications to all the devices on the network. If the network communication fails for any reason, the **Checking Network** message will appear and remain on screen.

Likely causes of this failure:

1. No devices connected to the network.
2. A problem with one of the devices.
3. Cable issue causing the entire network to fail.

Check the connections of the devices or try removing one device at a time from the system to isolate the problem device.

NOTE: Always turn off the system power before connecting or disconnecting any devices.

8.2. Startup Override

A system maintenance mode may be accessed to correct system issues. Enter the maintenance mode by pressing the handheld controller click wheel while system power is activated. Continue pressing the handheld controller click wheel until the **Startup Override** screen appears.

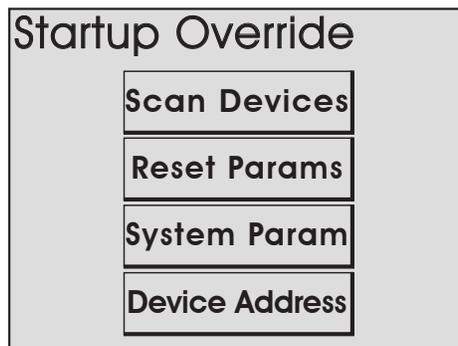


Fig. 240 - Startup override screen

8.2.1. Scan Devices

This utility scans the system network for devices. All possible device addresses and speeds are scanned. As devices are found, the address of the device and speed are displayed. When the scanning is complete, power to the system must be cycled.

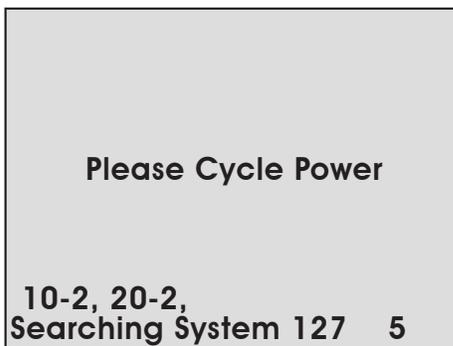


Fig. 241 - Cycle power screen

When a device is connected to the system but is not detected, this most likely indicates an internal device problem.

Normal network speeds will be **2** for all devices. When a device is not operating at the correct speed the internal software attempts to correct the device speed.

When a device is not operating at the correct speed, it may disrupt communications of the system network. Power should be cycled and the scan restarted.

TIP: *Within normal operation, issues with device speed will be very rare. Device network speeds are set by the manufacturer and should not deviate.*

8.2.2. Reset Parameters

If the system parameters become corrupt or a change is made that prevents the system from functioning properly. All system parameters may be restored to their factory settings by selecting this option. When pressing the **Reset Params** button, the changes occur immediately. Power will need to be cycled for the reset to be complete.

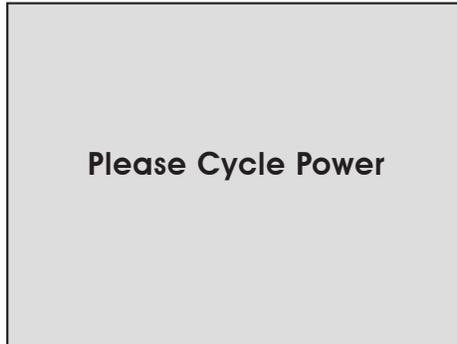


Fig. 242 - Cycle power screen

8.2.3. System Parameters

System parameters are factory set to control a variety of functions. These parameters can not be modified. However, special circumstances may occur when modification of these parameters could be recommended by the manufacturer.

Instructions for making changes to the system parameters will only be provided when deemed necessary by the manufacturer.

8.2.4. Device Address

Instructions for making changes to the system parameters will only be provided when deemed necessary by the manufacturer.

8.3. Additional Issues

Problem	Possible Cause	Solution
Handheld controller display does not activate	Input power requirements not met.	Ensure input power meets requirements. (see <i>"Power Requirements"</i> on page 10)
	Handheld controller not plugged into power controller.	Plug handheld controller into power controller. Ensure connectors are dry, clean and connector pins are not bent.
	Umbilical cable not properly connected.	Check umbilical cable connections at both ends. Ensure connectors are dry, clean and connector pins are not bent.
	SKOOT system not started.	Start the SKOOT system. (see <i>"System Startup"</i> on page 92)
	Damaged components in controller, crawler, power controller or cabling.	Contact manufacturer. (see <i>"Jireh Industries Ltd."</i> on page 3)
Handheld controller display is activated, yet crawler does not drive	Handheld controller is not in correct mode for driving.	(see <i>Operation</i> on page 97 for additional details).
	Damaged components in handheld controller, crawler, power controller or cabling.	Contact manufacturer. (see <i>"Jireh Industries Ltd."</i> on page 3)
Crawler does not drive and is unreachable	See possible causes for problem one of this list.	See solutions for problem one. If the crawler is still unresponsive (see <i>"Retrieval of a Stranded Crawler"</i> on page 118)

For technical assistance (see *"Technical Support"* on page 119)

8.4. Retrieval of a Stranded Crawler



WARNING! FALLING OBJECT HAZARD.

The tether system must remain active while retrieving the crawler (*i.e. a mechanism or person must be continuously taking up the slack in the tether*).

Should the **SKOOT** crawler become inoperative while out of reach, attempt first, the solutions offered in this manual (*see "Troubleshooting" on page 113*)

If troubleshooting does not rectify the issue, it may be necessary to retrieve the crawler manually. To do so:

1. Press the E-Stop push-button turning crawler power off.

NOTE: *Under normal conditions, the crawler should begin descending slowly.*

2. If the crawler stops descending due to some kind of impediment, use a ladder, man lift or scaffolding to assist the crawler in overcoming the obstacle.

NOTE: FALLING OBJECT HAZARD. *It is **CRUCIAL** that the tether system remains active while retrieving the crawler (*i.e. a mechanism or person must be continuously taking up slack in the tether*).*

SERVICE AND REPAIR



WARNING! ELECTRICAL SHOCK HAZARD. Disconnect the power controller when servicing the equipment. The power controller is powered even when the E-Stop push-button is latched in the off position.



WARNING! MAGNETIC MATERIAL. The wheels of the crawler produce an extremely strong magnetic field which may cause failure or permanent damage to items such as watches, memory devices, CRT monitors, medical devices or other electronics.

Tools, magnets and metal objects can cut, pinch or entrap hands and fingers. **HANDLE WITH CARE.**

Those with pacemakers or ICD's must stay at least 25 cm (10 in) away at all times.



WARNING! DO NOT DISASSEMBLE. No user-serviceable parts. Disassembling any of the components in this product, beyond the instructions in this user manual, could void the regulatory certifications and/or effect the safety of the product.

9.1. Technical Support


For technical support contact Jireh Industries (see "Jireh Industries Ltd." on page 3).

SPARE PARTS

To order accessories or replacement parts for your **SKOOT** system.
 (contact Jireh Industries Ltd. on page 3)

NOTE: These drawings are for parts order. This is not a list of kit contents.


10.1. SKOOT Crawler

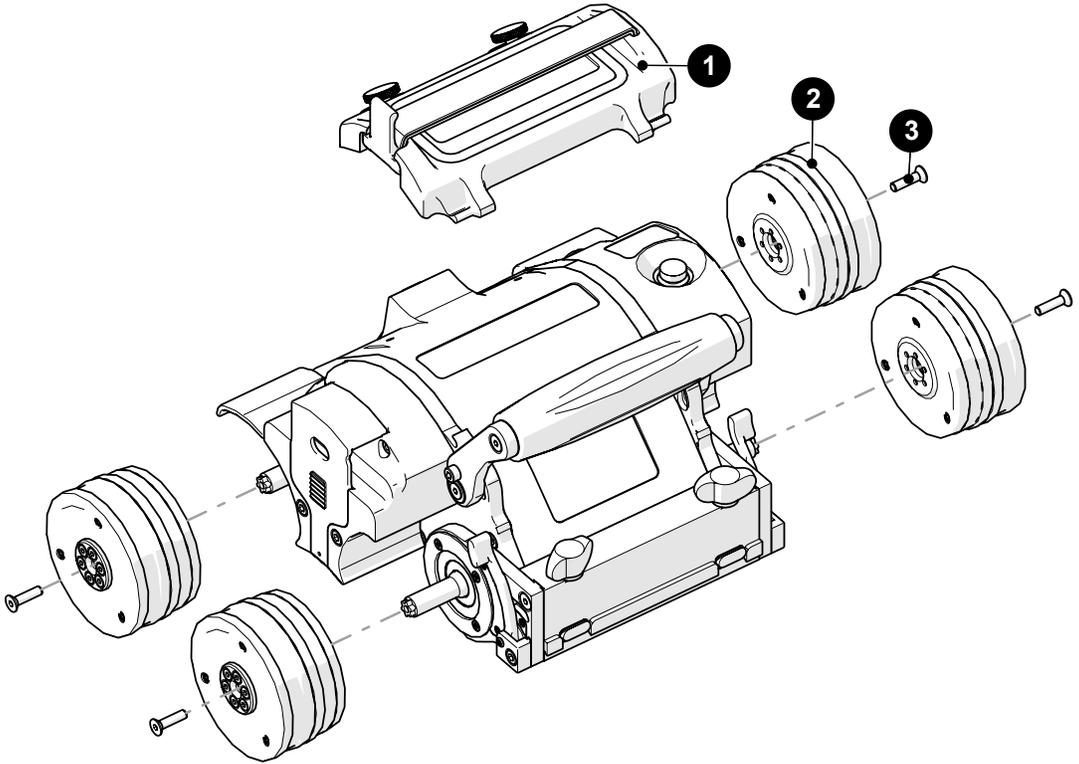

BOM ID	Part #	Description
1	DNS008	Backpack
2	CXS005	Magnetic Wheel
3	MD029-016	FHCS, M4x0.7 X 12 mm, SST

Fig. 243 - SKOOT base crawler spare parts

10.2. SKOOT Kit Components

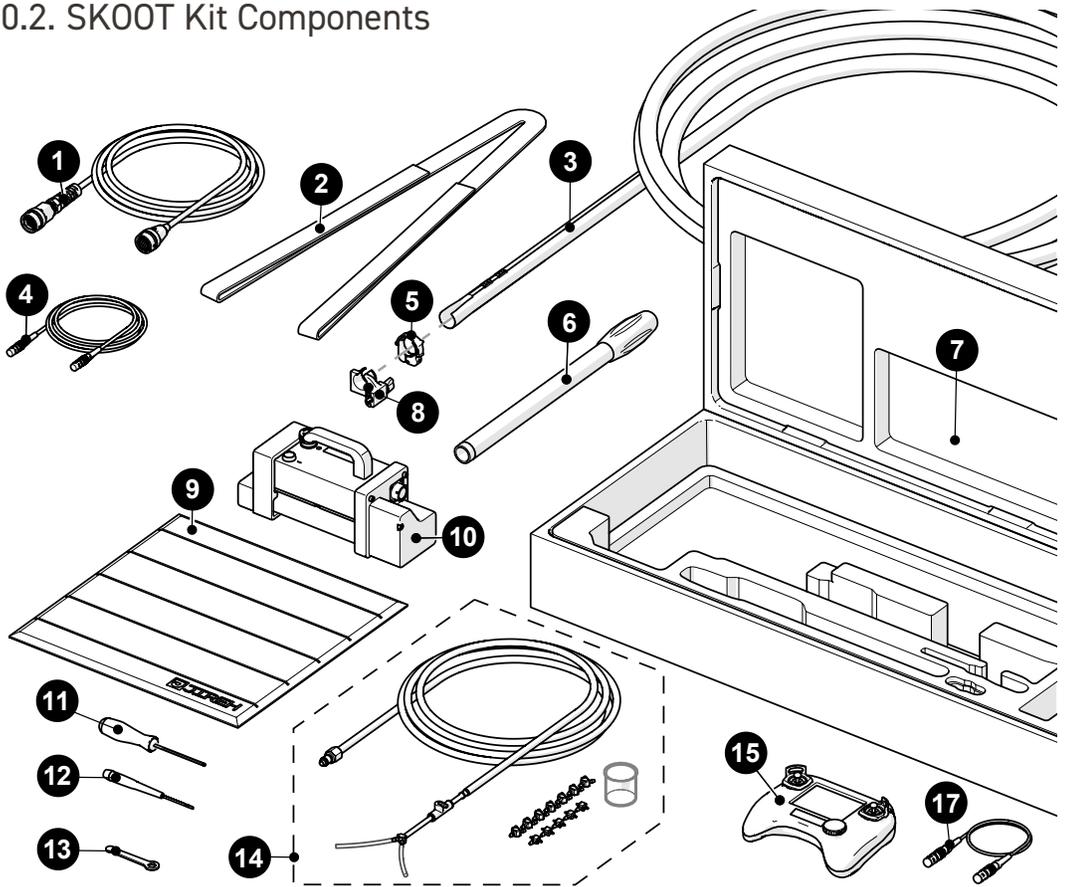

BOM ID	Part #	Description
1	UMA022-X	Umbilical (<i>various lengths available</i>)
2	EA243	Sling
3		<i>See Cable Management Sleeving</i>
4	UMA017-06	Auxiliary Cable
5	CES066	Cable Management Clamp
6	DNS006	Manipulation Handle
7	DNA008	SKOOT Case
8	CXS073	Cable Management Mount
9	AAS061	Installation/Removal Mat
10	DNA006-X	SKOOT Power Controller (<i>See Power Cord Type</i>)
11	EA414	3 mm (<i>0.118 in</i>) Hex Driver
12	EA480	3 mm (<i>0.118 in</i>) Flat Driver
13	EA470	10 mm (<i>3/8 in</i>) Wrench
14	CMG009-X	Irrigation Kit, 2-4 Probe, Large Tube (<i>Various lengths available</i>)
15	CXA008	Handheld Controller
16	UMA025-X-05	J300 Encoder Cable (<i>see Encoder Connector Type</i>)

Fig. 244 - Kit components spare parts

10.2.1. Encoder Connector Type

Connector Type	Company/Instrument	Connector Type	Company/Instrument
B	Olympus - OmniScan MX / Zetec - ZIRCON, TOPAZ	G	Sonotron - Isonic
C	Olympus - Focus LT / Zetec Z-Scan / Eddyfi Ectane 2	M	GE - USM Vision
D	Olympus - OmniScan MX2, OmniScan SX	U	Sonatest - VEO, PRISMA
F	TD - Focus Scan, Handy Scan, Pocket Scan	V	Pragma PAUT 16/128, PragmaLite / Pragma UT400

Fig. 245 - Encoder connector type


NOTE: Additional encoder connector types available.
(contact Jireh Industries Ltd. on page 3)

10.2.2. Power Cord Type

Connector Type	Power Cord	Connector Type/ Part #	Power Cord
N SL032	North American	U SL059	United Kingdom
E SL039	European	Z	No Cord

Fig. 246 - Encoder connector type


10.3. Probe Holder Frame

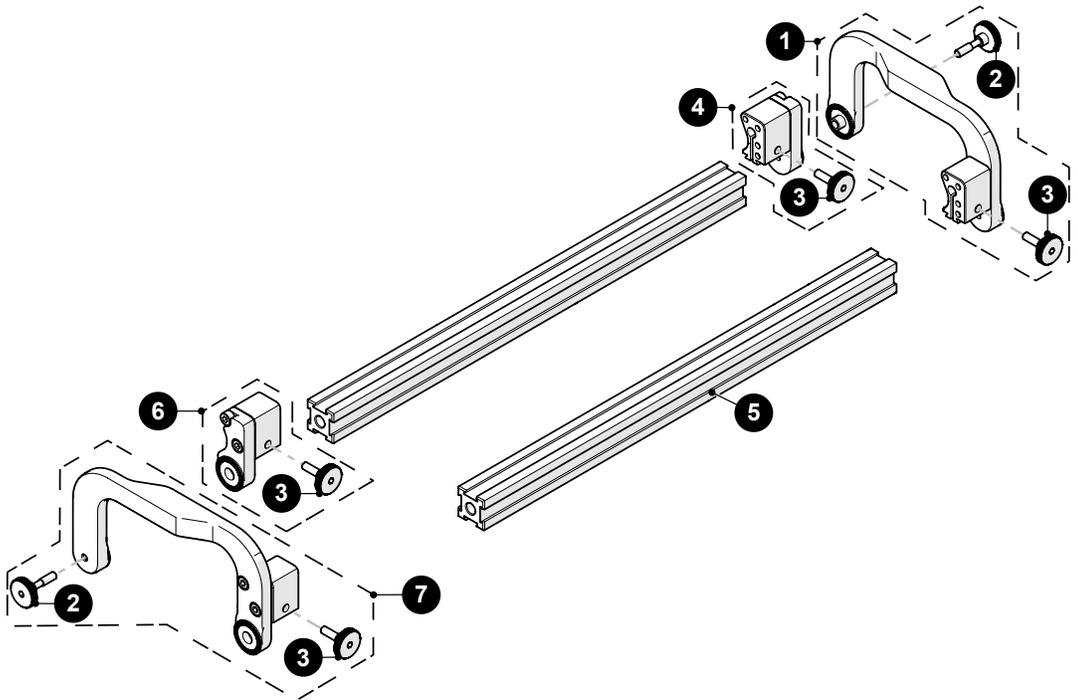

BOM ID	Part #	Description
1	CXS043	Vertical Probe Holder Side Arm, Left
2	CX0125	Knob, M4 x 16 mm
3	CX0126	Knurled Knob, M4 x 0.7 x 11.5 mm, 3 mm hex, 4 mm stand off, SST
4	CXS072-L	Arm Mount Block, Left
5	BG0038-X	Frame Bar (see <i>Frame Bar</i>)
6	CXS072-R	Arm Mount Block, Right
7	CXS042	Vertical Probe Holder Side Arm, Right

Fig. 247 - Probe holder frame parts


10.4. Low Profile Probe Holder Frame

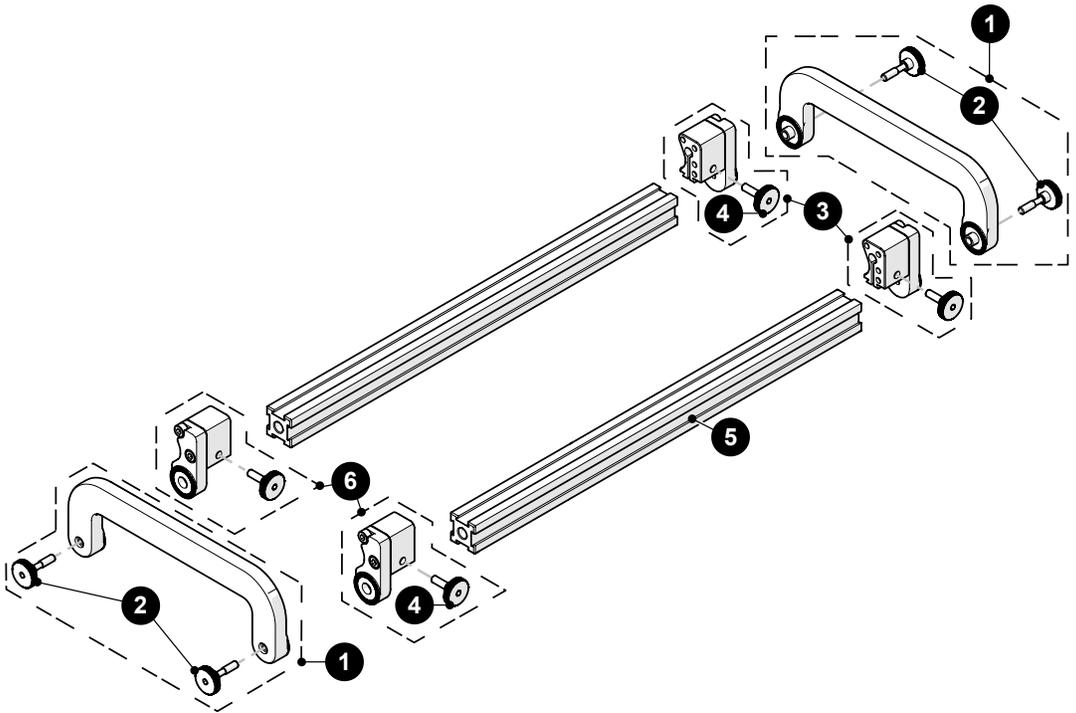

BOM ID	Part #	Description
1	CXS023	Low Profile Side Arm
2	CX0125	Knob, M4 x 16 mm
3	CXS072-L	Arm Mount Block, Left
4	CX0126	Knurled Knob, M4 x 0.7 x 11.5 mm, 3 mm hex, 4 mm stand off, SST
5	BG0038-X	Frame Bar (<i>see Frame Bar</i>)
6	CXS072-R	Arm Mount Block, Right

Fig. 248 - Low profile probe holder frame parts


10.5. Pivoting Probe Holder Frame

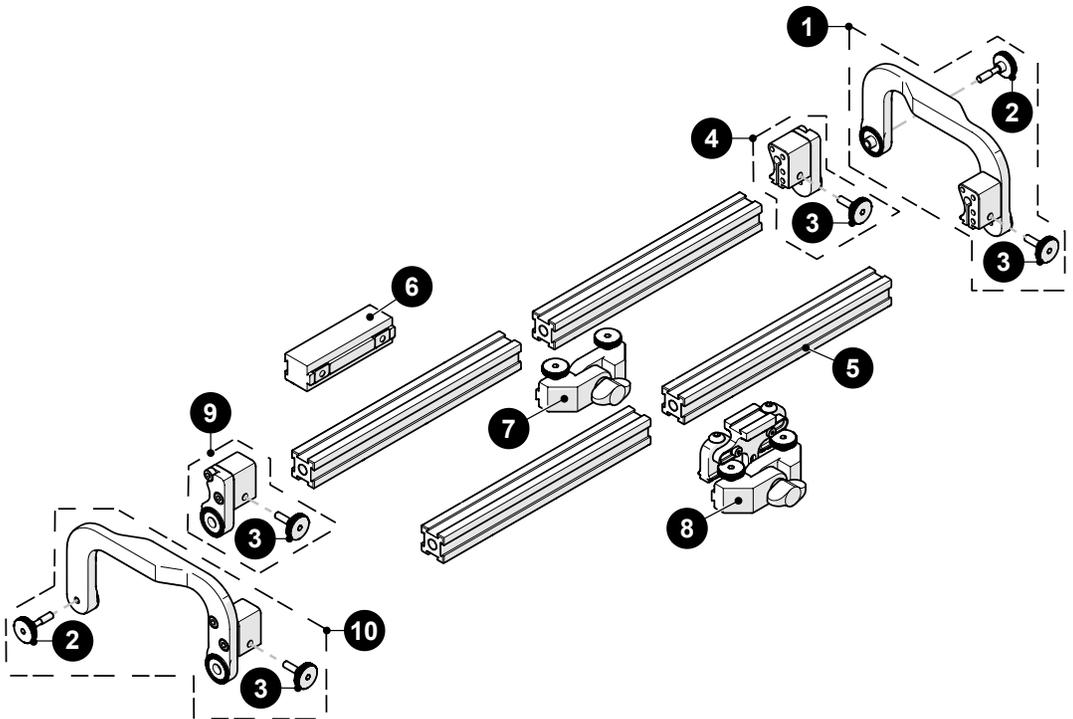

BOM ID	Part #	Description
1	CXS043	Vertical Probe Holder Side Arm, Left
2	CX0125	Knob, M4 x 16 mm
3	CX0126	Knurled Knob, M4 x 0.7 x 11.5 mm, 3 mm hex, 4 mm stand off, SST
4	CXS072-L	Arm Mount Block, Left
5	BG0038-X	Frame Bar (<i>see Frame Bar</i>)
6	CXS064	NAVIC Front Spacer Mount
7	CXS055	Frame Bar Pivot
8	CXS059	Optical Guide Pivot Mount
9	CXS072-R	Arm Mount Block, Right
10	CXS042	Vertical Probe Holder Side Arm, Right

Fig. 249 - Pivoting probe holder parts


10.6. Slip Joint Probe Holder Parts

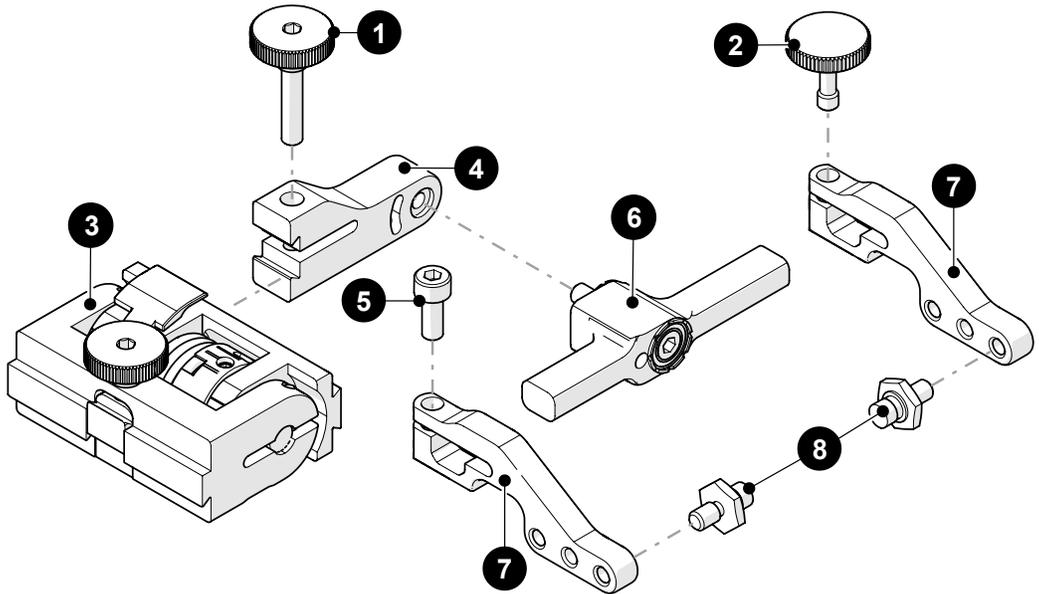

BOM ID	Part #	Description
1	PH0104	Knurled Knob, M4 x 0.7 x 18 mm, 4 mm stand off, SST
2	PH0082	Knurled Knob, M4 x 0.7 x 10 mm, 3 mm stand off, SST
3	PHS022	Slip Joint Probe Holder Subassembly
4		<i>see Swing Arm Style</i>
5	MD050-010	SHCS, M4 x 0.7 x 10 mm, SST
6		<i>see Yoke Style</i>
7		<i>see Arm Style</i>
8	PH0011-X	Pivot Button Style (<i>see Pivot Button Style</i>)

Fig. 250 - Slip joint probe holder parts


10.7. Vertical Probe Holder Parts

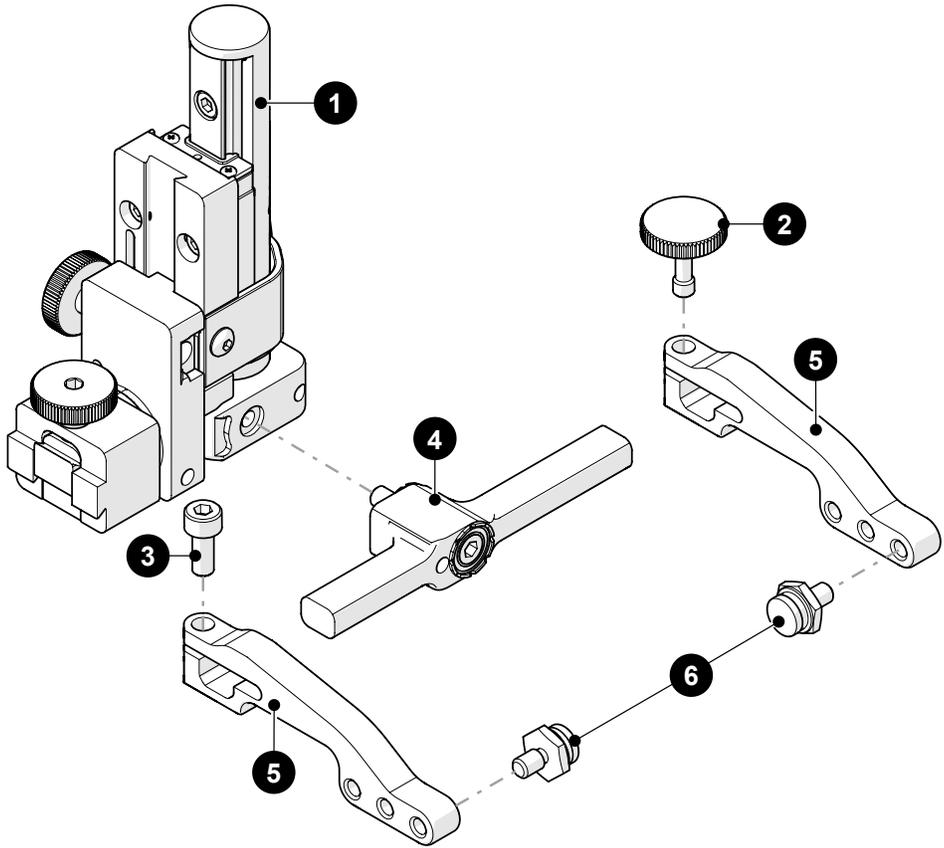

BOM ID	Part #	Description
1	PHS028	Vertical Probe Holder Subassembly
2	PH0082	Knurled Knob, M4 x 0.7 x 10 mm, 3 mm stand off, SST
3	MD050-010	SHCS, M4 x 0.7 x 10 mm, SST
4		see Yoke Style
5		see Arm Style
6	PH0011-X	Pivot Button Style (see Pivot Button Style)

Fig. 251 - Vertical probe holder parts


10.8. Heavy Duty Vertical Probe Holder

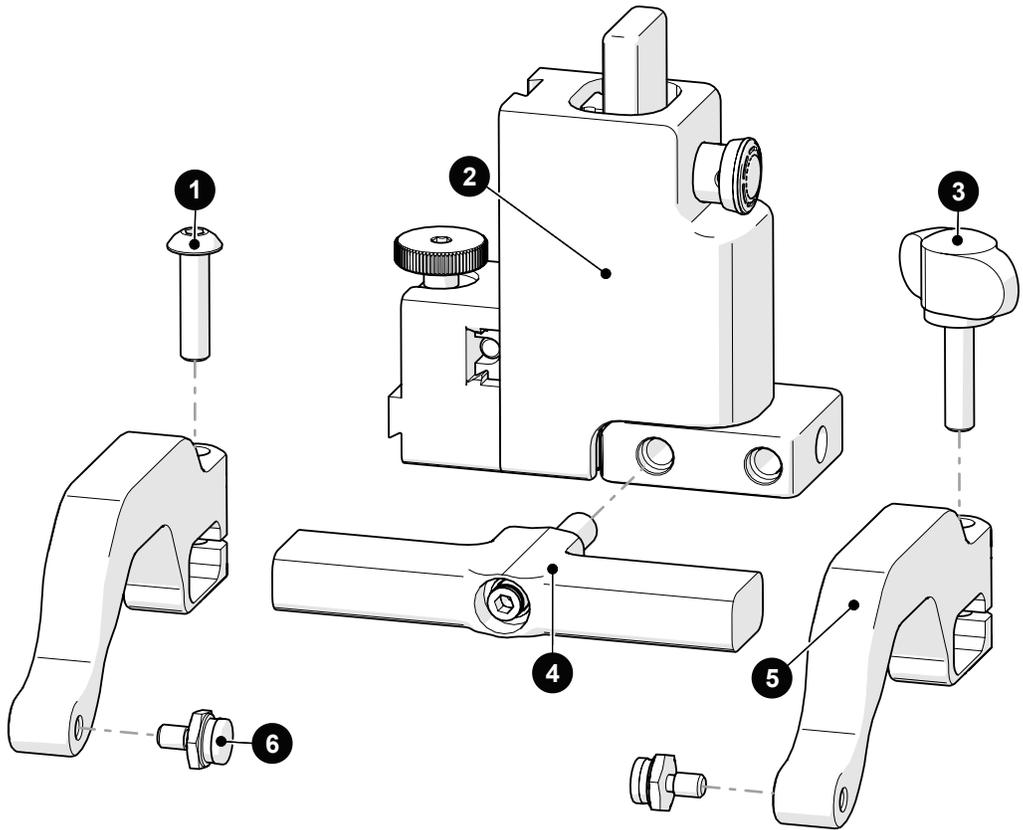

BOM ID	Part #	Description
1	MD074-020	BHCS, M5 x 0.8 x 20 mm, SST
2	PHS049	Heavy Duty Probe Holder Subassembly
3	EA154	Probe Holder Arm Adjustment Knob
4	<i>See Heavy Duty Yoke Style</i>	
5	PH0165	Heavy Duty Probe Holder Arm, Standard, Drop
6	PH0011-X	Pivot Button Style (<i>See Pivot Button Style</i>)

Fig. 252 - Heavy duty vertical probe holder parts

10.9. Corrosion Thickness Probe Holder

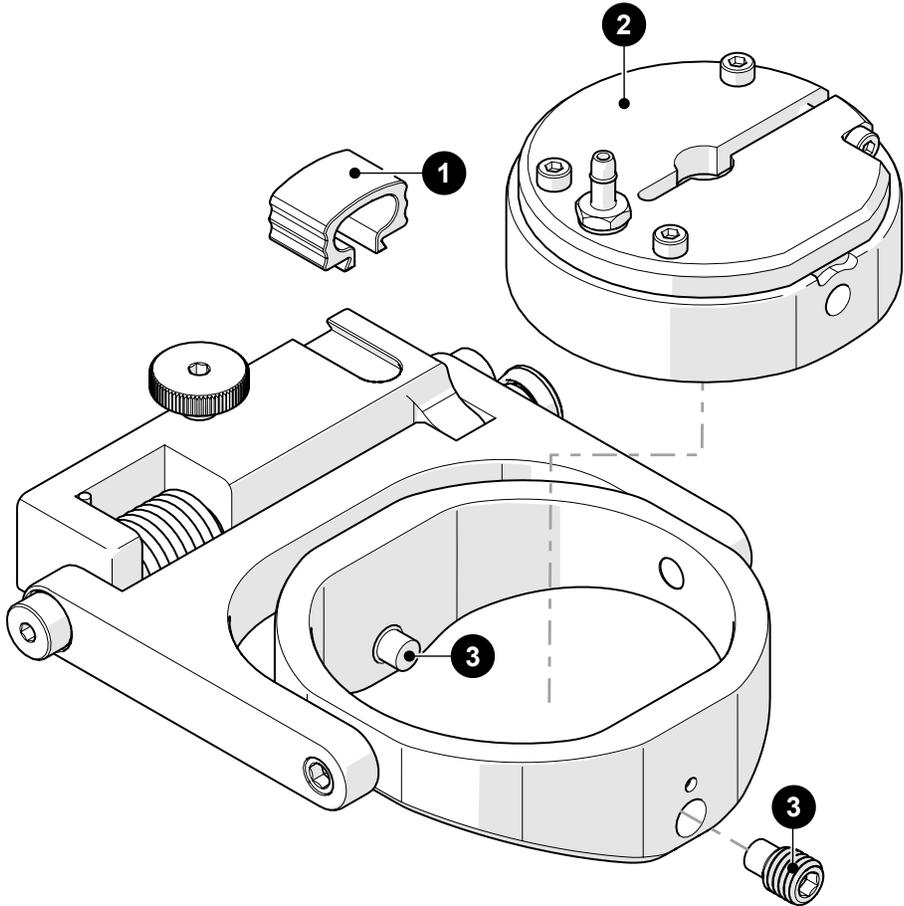

BOM ID	Part #	Description
1	BG0091	Cable Clip
2	<i>See Probe Holder Receptacle and Wear Plate</i>	
3	MA264	SHSS, M8 x 1.25 x 12 mm, dog point, SST

Fig. 253 - Corrosion thickness probe holder parts

10.10. Probe Holder Components

10.10.1. Arm Style

Arm Style	Part #		Arm Style	Part #	
A Standard, Flat	PH0090		B Short, Flat	PH0089	
C Long, Flat	PH0099		D Standard, Drop	PH0093	
E Short, Drop	PH0092		F Long, Drop	PH0094	
G Standard, Extra-Drop	PH0096		H Short, Extra-Drop	PH0095	
I Extra-Short, Flat	PH0159		J Extra-Short, Drop	PH0161	

Fig. 254 - Probe holder arm selection

10.10.2. Yoke Style

Yoke Style	Part #	Length		Yoke Style	Part #	Length	
S Standard	PHS052	6.3 cm (2.47 in)		W Wide	PHS063	7.9 cm (3.06 in)	

Fig. 255 - Probe holder yoke selection

10.10.3. Swing Arm Style

Swing Arm Style	Part #	Length		Swing Arm Style	Part #	Length	
Short	PH0069	4.1 cm (1.61 in)		Long	PH0100	4.6 cm (1.81 in)	

Fig. 256 - Swing arm selection

10.10.4. Heavy Duty Yoke Style

Yoke Style	Part #	Length		Yoke Style	Part #	Length	
S Standard	PHS048	8.3 cm (3.26 in)		W Wide	PHS047	12.2 cm (4.79 in)	

Fig. 257 - Heavy duty probe holder yoke selection

10.10.5. Pivot Button Style

Pivot Hole Size	Wedge Type		Pivot Hole Size	Wedge Type	
01 8.0 mm (0.32 in)	Olympus PA		02 5.0 mm (0.20 in)	Olympus TOFD	
03 2.7 mm (0.11 in)	Sonatest DAAH PA		04 9.5 mm (0.38 in)	-	
06 3.0 mm (0.12 in)	-		07 2.3 mm (0.09 in)	-	
08 Conical Head	-		09 5 mm (0.20 in) Internal	Zetec PA/TOFD	

Fig. 258 - Pivot button selection

NOTE: Additional probe holder pivot button types available.
(see "Jireh Industries Ltd." on page 3)

10.10.6. Probe Holder Receptacle and Wear Plate

Part #	Wear Plate	Receptacle	Part #	Wear Plate	Receptacle
PHS066-A	Curved	9.53 mm (0.375 in) dia.	PHS066-B	Curved	12.7 mm (0.5 in) dia.
PHS066-C	Curved	19 mm (0.75 in) dia.	PHS066-E	Curved	25.4 mm (1 in)
PHS067-A	Flat	9.53 mm (0.375 in) dia.	PHS067-B	Flat	12.7 mm (0.5 in) dia.
PHS067-C	Flat	19 mm (0.75 in) dia.	PHS067-D	Flat	Technisonic
PHS067-E	Flat	25.4 mm (1 in)			

Fig. 259 - Pivot button selection

10.11. Variable Components

10.11.1. Frame Bar

Part #	Length	Part #	Length
BG0038-05	5 cm (1.97 in)	BG0038-10	10 cm (3.94 in)
BG0038-15	15 cm (5.91 in)	BG0038-20	20 cm (7.87 in)
BG0038-25	25 cm (9.84 in)	BG0038-30	30 cm (11.81 in)
BG0038-35	35 cm (13.78 in)	BG0038-40	40 cm (15.75 in)
BG0038-45	45 cm (17.72 in)	BG0038-50	50 cm (19.69 in)
BG0038-55	55 cm (21.65 in)		

Fig. 260 - Frame bar selection


10.11.2. Cable Management Sleeving

Part #	Length
CX0141	4.5 m (14.8 ft)
CX0145	9.5 m (31.2 ft)
CX0146	14.5 m (47.6 ft)
CX0147	29.5 m (96.8 ft)

Fig. 261 - Cable management sleeving

10.12. Accessories

10.12.1. Automated Crawler Medium Temperature Add-On Kit

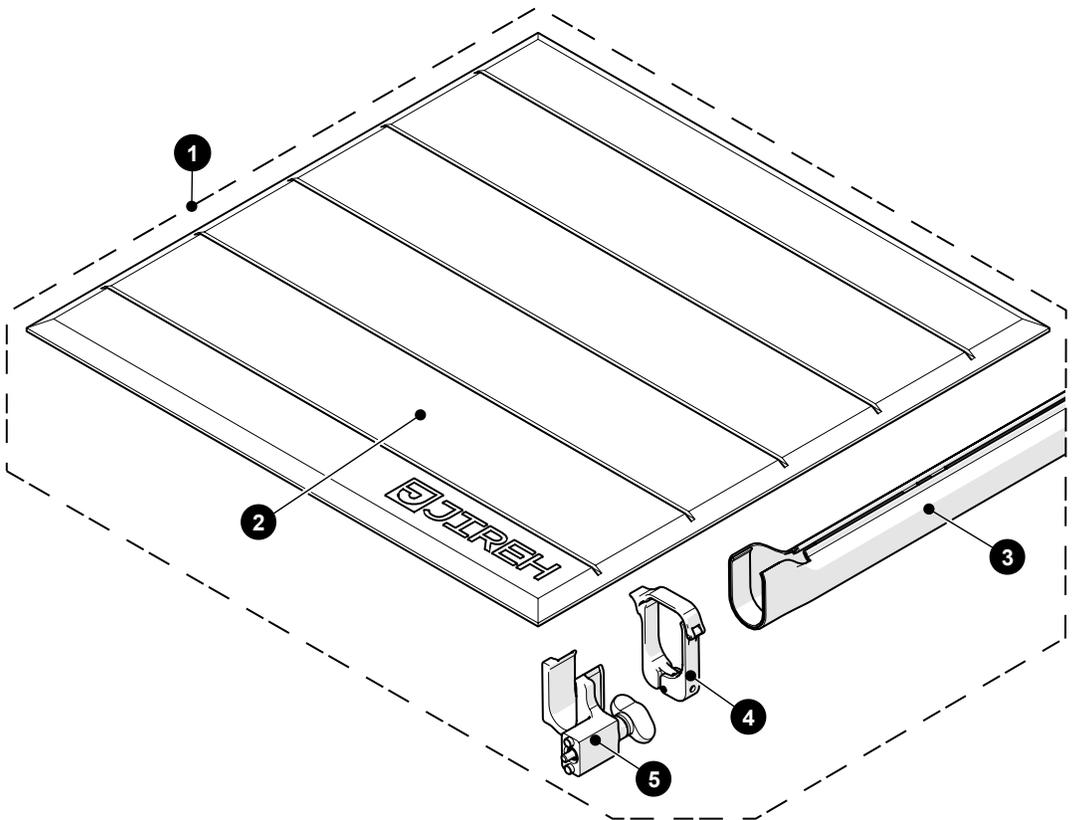

BOM ID	Part #	Description
1	CXG031-04.5	Automated Crawler Medium Temperature Add-On Kit
2	CXS102	Medium Temperature Installation/Removal Mat
3	CX0371-04.5	Medium Temperature Sleeve
4	CXS114	Medium Temperature Clamp
5	CXS112	Medium Temperature Mount

Fig. 262 - Automated Crawler Medium Temperature Add-On Kit

10.12.2. Preamp Bracket

Part #	Description
CES029	Preamp Bracket
CES029-V	Preamp Bracket with Velcro


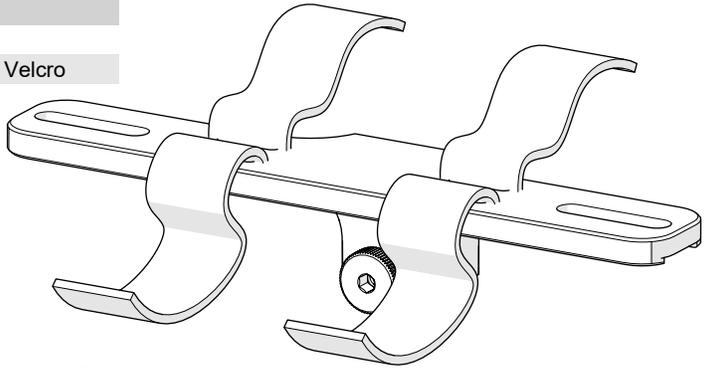


Fig. 263 - Preamp bracket


10.12.3. Battery Powered Optical Guide

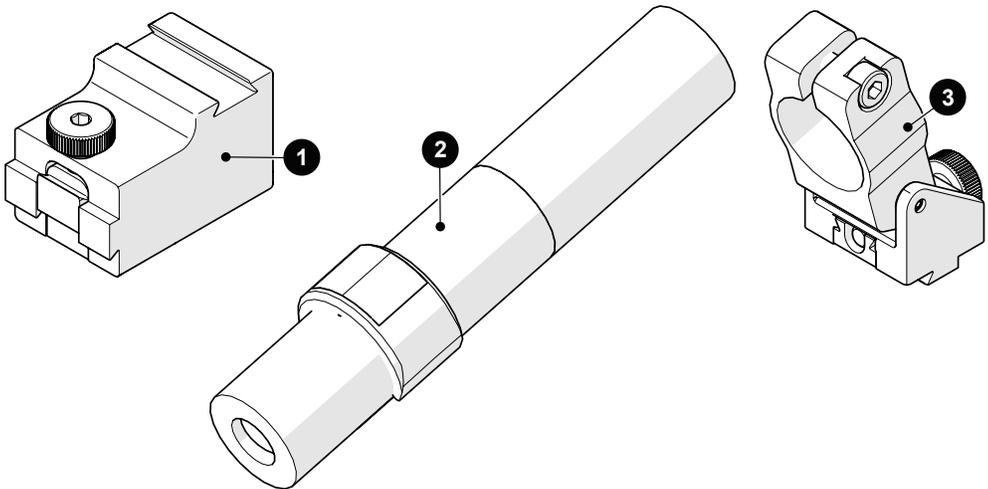

BOM ID	Part #	Description
1	BGS068	Perpendicular Dovetail Mount
2	JV024	Line Laser, Battery Powered, Class 1
3	CXS082	Optical Guide Clamp

Fig. 264 - Battery powered optical guide

10.13. Cases

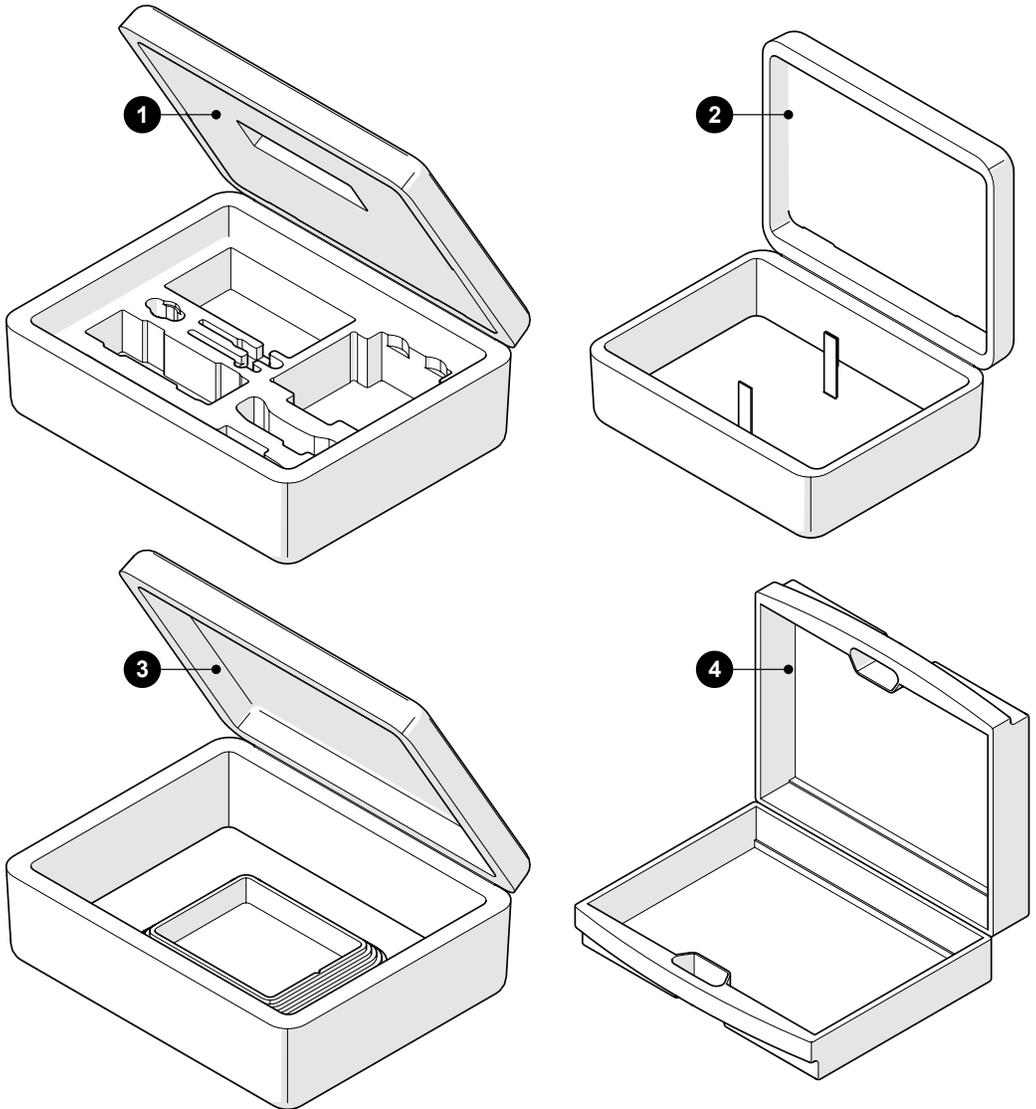


BOM ID	Part #	Description
1	DNA010	SKOOT Crawler Case
2	CXA023	Umbilical / Probe Holder Frame Case
3	CMA016	Motorized Pump / Umbilical Case
4	EA421	Umbilical Case

Fig. 265 - Cases

DISPOSAL

WEEE Directive

In accordance with European Directive on Waste Electrical and Electronic Equipment (WEEE), this symbol indicated that the product must not be disposed of as unsorted municipal waste, but should be collected separately. Refer to Jireh Industries for return and/or collection systems available in your country.



LIMITED WARRANTY

WARRANTY COVERAGE

Jireh Industries warranty obligations are limited to the terms set forth below: Jireh Industries Ltd. (“Jireh”) warrants this hardware product against defects in materials and workmanship for a period of THREE (3) YEARS from the original date of purchase. If a defect exists, at its option Jireh will (1) repair the product at no charge, using new or refurbished replacement parts, (2) exchange the product with a product that is new or which has been manufactured from new or serviceable used parts and is at least functionally equivalent to the original product, or (3) refund the purchase price of the product. A replacement product/part assumes the remaining warranty of the original product or ninety (90) days from the date of replacement or repair, whichever provides longer coverage for you. When a product or part is exchanged, any replacement item becomes your property and the replaced item becomes Jireh’s property. When a refund is given, your product becomes Jireh’s property.

OBTAINING WARRANTY SERVICE

To utilize Jireh’s warranty service you must ship the product, at your expense, to and from Jireh Industries. Before you deliver your product for warranty service you must phone Jireh and obtain an RMA number. This number will be used to process and track your product. Jireh is not responsible for any damage incurred during transit.

EXCLUSIONS AND LIMITATIONS

This Limited Warranty applies only to hardware products manufactured by or for Jireh Industries. This warranty does not apply: (a) to damage caused by accident, abuse, misuse, misapplication, or non-Jireh products; (b) to damage caused by service (including upgrades and expansions) performed by anyone who is not a Jireh Authorized Service Provider; (c) to a product or a part that has been modified without the written permission of Jireh.

Jireh Industries Ltd.
53158 Range Road 224
Ardrossan AB T8E 2K4
Canada
Phone: 780-922-4534
jireh.com

HydroFORM™ is a trademark of Olympus

All brands are trademarks or registered trademarks of their respective owners and third party entities.

Changes or modifications to this unit or accessories, not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

All specifications are subject to change without notice.

© 2015 - 2020 Jireh Industries Ltd.



Jireh Industries Ltd.
53158 Range Road 224
Ardrossan, Alberta
Canada
T8E 2K4

780-922-4534

jireh.com